


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091218\
Data File : VU026675.D
Acq On : 11 Sep 2018 10:04
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Title : SW846 8260
Last Update : Wed Sep 12 05:32:45 2018

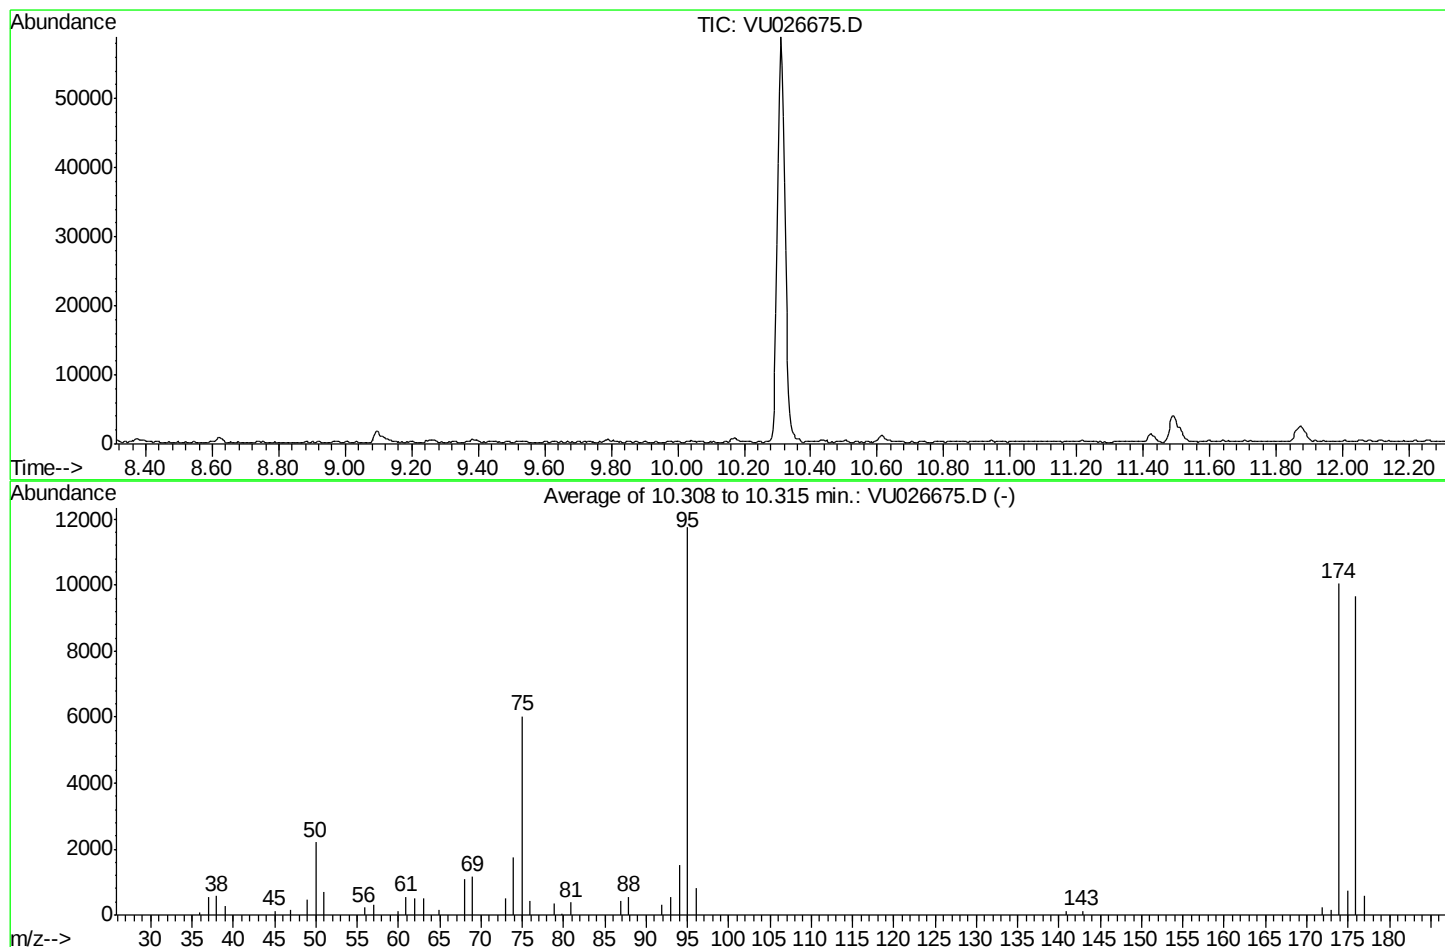

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	2211	PASS
75	95	30	60	51.2	6018	PASS
95	95	100	100	100.0	11755	PASS
96	95	5	9	6.8	797	PASS
173	174	0.00	2	1.7	166	PASS
174	95	50	100	85.4	10043	PASS
175	174	5	9	7.2	725	PASS
176	174	95	101	96.3	9667	PASS
177	176	5	9	6.2	602	PASS