

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
 Data File : VU055270.D
 Acq On : 13 Sep 2023 04:15
 Operator : MD/SY
 Sample : 04350-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 13 05:37:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 13 05:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.248	114	178848	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	187968	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	84008	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	26799	3.197	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.000%
7) Chloroethane-d5	1.907	69	40811	4.206	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.200%
11) 1,1-Dichloroethene-d2	2.563	65	15121	3.166	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.400%
20) 2-Butanone-d5	4.624	46	135483	55.698	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.400%
24) Chloroform-d	5.062	84	99188	4.459	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
26) 1,2-Dichloroethane-d4	5.698	65	52047	4.677	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%
32) Benzene-d6	5.724	84	182667	3.937	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.800%
36) 1,2-Dichloropropane-d6	6.689	67	61621	4.176	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.600%
41) Toluene-d8	7.898	98	158383	3.706	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.200%
43) trans-1,3-Dichloroprop...	8.181	79	13938	3.430	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.600%
46) 2-Hexanone-d5	8.631	63	76213	46.192	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.380%
56) 1,1,2,2-Tetrachloroeth...	10.756	84	47382	4.565	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.400%
66) 1,2-Dichlorobenzene-d4	12.193	152	52809	4.307	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.200%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.383	85	2723	0.262	ug/L #	85
3) Chloromethane	1.518	50	1478	0.140	ug/L	87
5) Vinyl chloride	1.602	62	114728	10.279	ug/L	98
10) 1,1,2-Trichloro-1,2,2-...	2.576	101	2693	0.285	ug/L #	84
12) 1,1-Dichloroethene	2.576	96	170646	20.638	ug/L #	75
17) Methyl tert-butyl Ether	3.361	73	94966	4.379	ug/L	99
18) trans-1,2-Dichloroethene	3.354	96	7339	0.875	ug/L	99
19) 1,1-Dichloroethane	3.866	63	72507	3.999	ug/L	97
22) cis-1,2-Dichloroethene	4.660	96	6939633	675.786	ug/L	92
25) Chloroform	5.084	83	55633	2.946	ug/L	92
27) 1,2-Dichloroethane	5.795	62	18313	1.589	ug/L	96
29) 1,1,1-Trichloroethane	5.316	97	16025	0.986	ug/L #	88
33) Benzene	5.772	78	5824	0.146	ug/L	100
34) Trichloroethene	6.541	95	2879494	258.990	ug/L	98
35) Methylcyclohexane	6.689	83	15370	0.985	ug/L #	34
37) 1,2-Dichloropropane	6.685	63	7646	0.702	ug/L #	90
45) 1,1,2-Trichloroethane	8.402	97	1060	0.144	ug/L #	60
47) Tetrachloroethene	8.553	164	23409	3.046	ug/L	95
48) 2-Hexanone	8.679	43	20216	4.154	ug/L #	87

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055270.D
Acq On : 13 Sep 2023 04:15
Operator : MD/SY
Sample : 04350-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 13 05:37:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 13 05:34:47 2023
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Dibromochloromethane	8.553	129	22284	2.783	ug/L #	9
61) 1,2,3-Trichloropropane	11.811	75	10796	1.937	ug/L #	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 13 05:37:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 13 05:34:47 2023
Response via : Initial Calibration




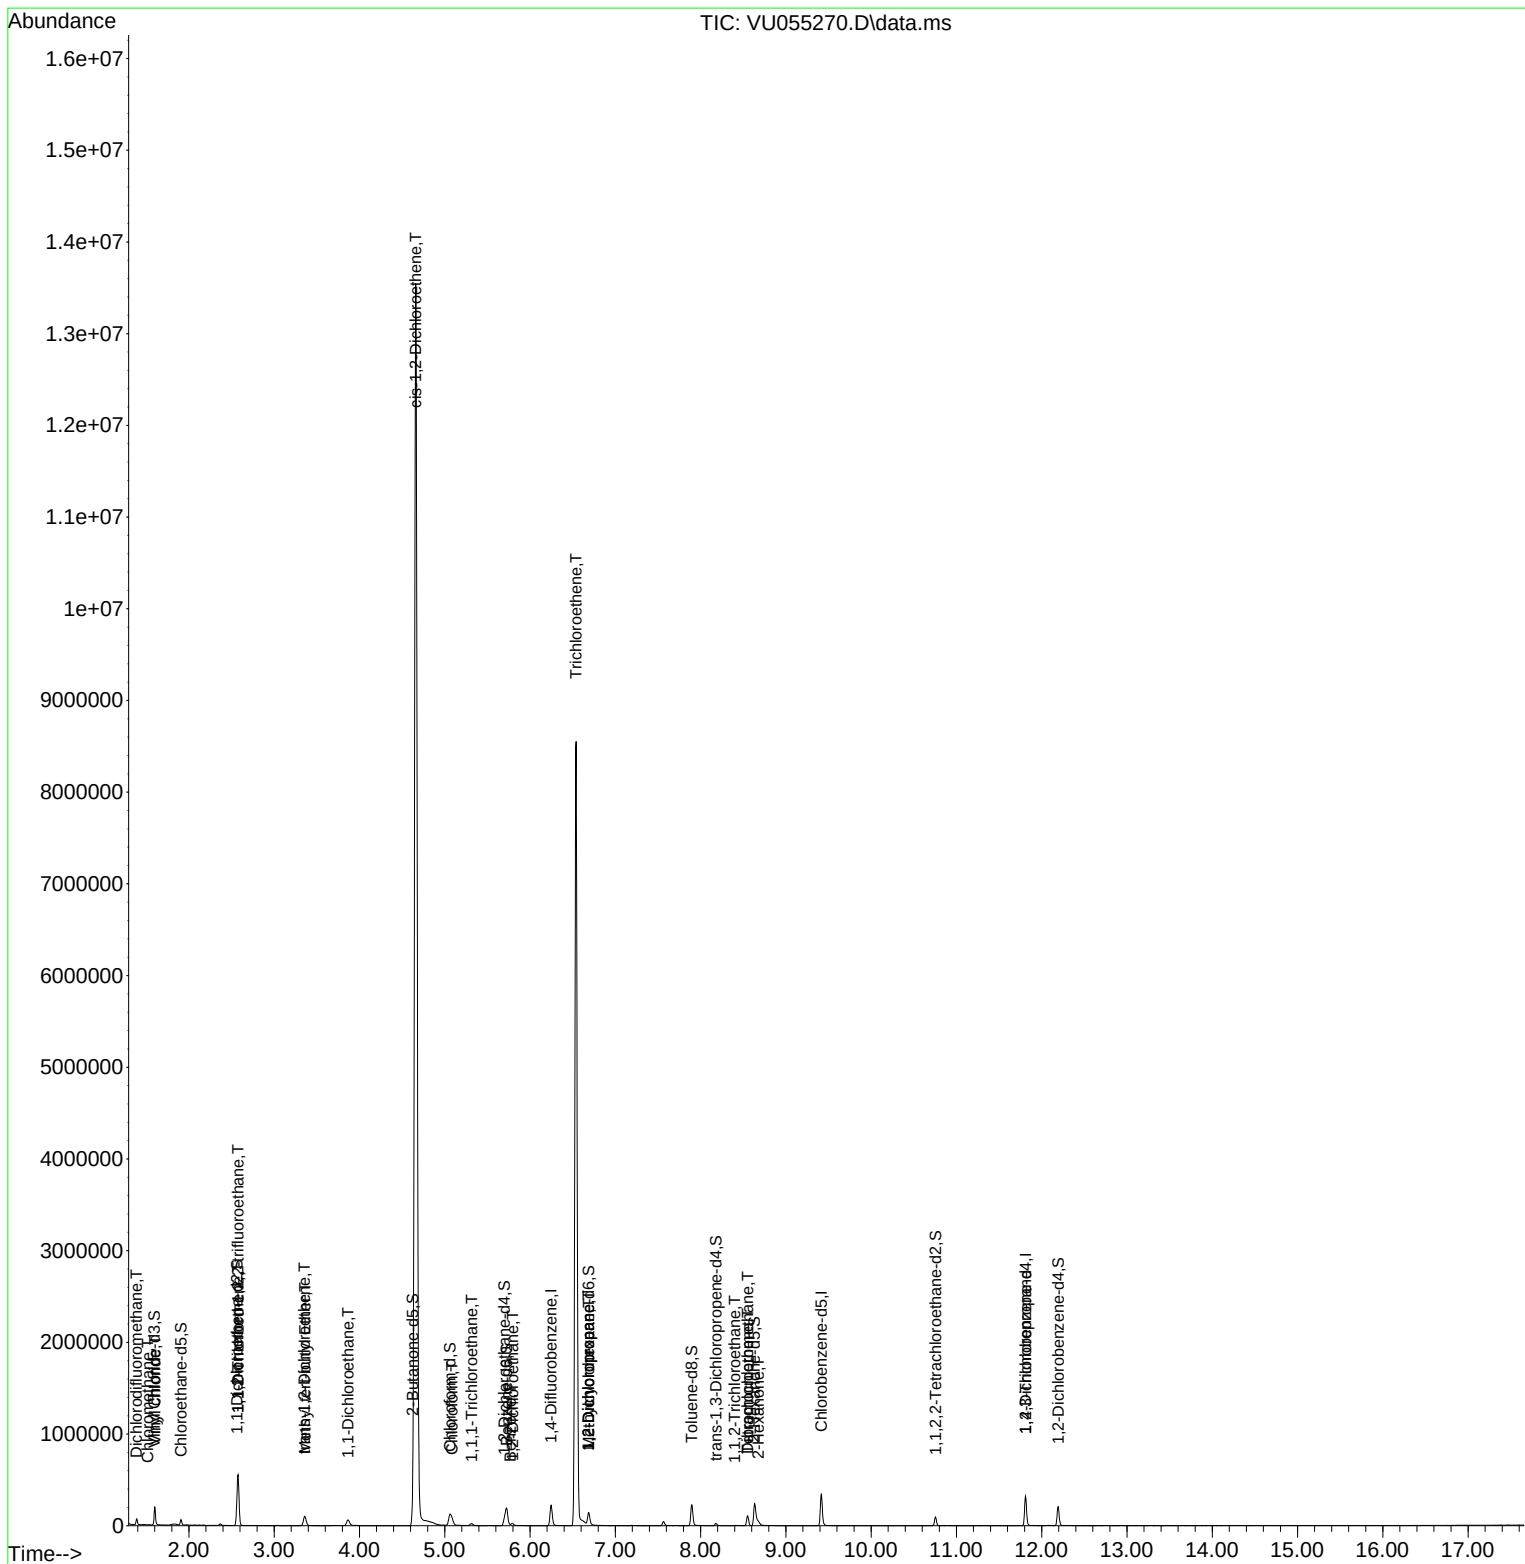


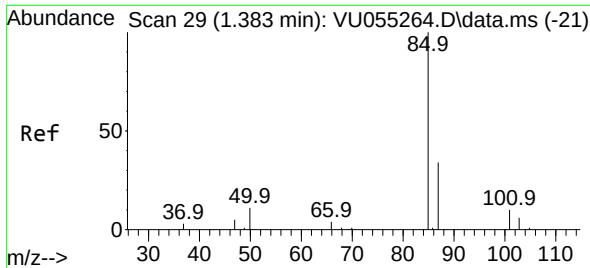

#2
 Dichlorodifluoromethane
 Concen: 0.262 ug/L
 RT: 1.383 min Scan# 29
 Delta R.T. 0.000 min
 Lab File: VU055270.D
 Acq: 13 Sep 2023 04:15




Instrument :
 MSVOA_U
 ClientSampleId :


Tgt Ion: 85 Resp: 2723
 Ion Ratio Lower Upper
 85 100
 87 39.7 25.1 37.7#

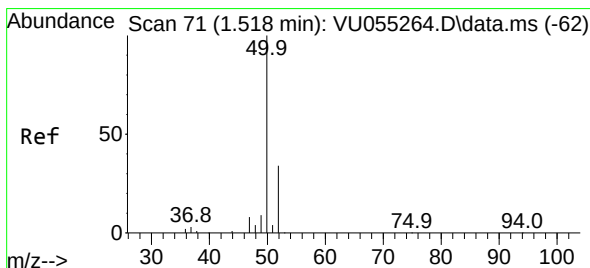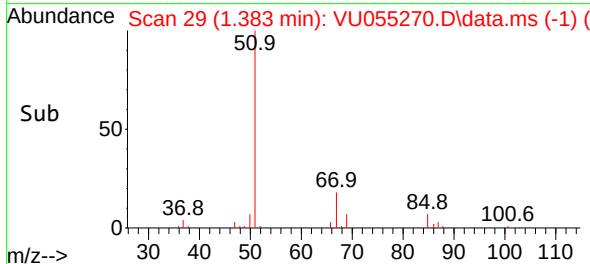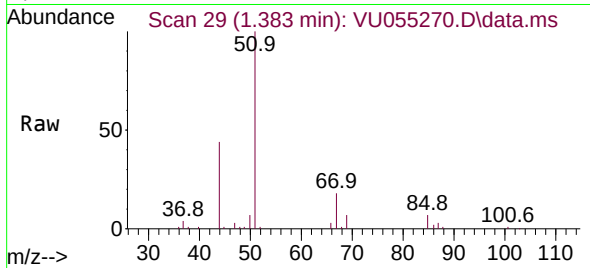

#3
 Chloromethane
 Concen: 0.140 ug/L
 RT: 1.518 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: VU055270.D
 Acq: 13 Sep 2023 04:15

Tgt Ion: 50 Resp: 1478
 Ion Ratio Lower Upper
 50 100
 52 39.1 22.5 41.7


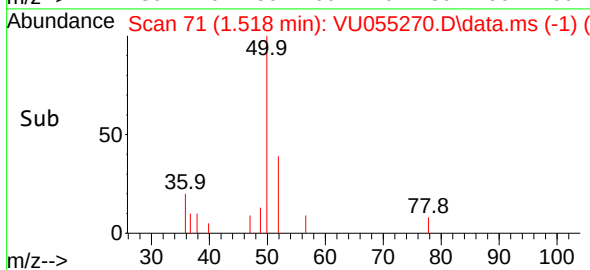

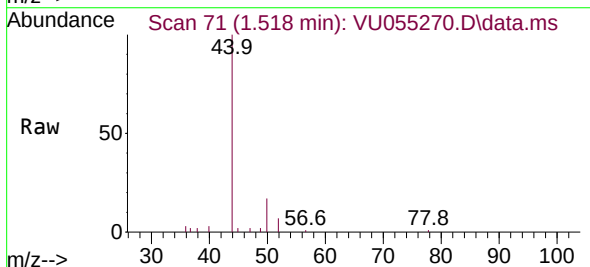


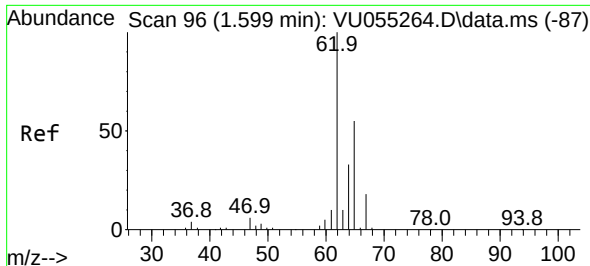

#5
 Vinyl chloride
 Concen: 10.279 ug/L
 RT: 1.602 min Scan# 91
 Delta R.T. 0.003 min
 Lab File: VU055270.D
 Acq: 13 Sep 2023 04:15




Instrument :
 MSVOA_U
 ClientSampleId :


Tgt Ion: 62 Resp: 114728
 Ion Ratio Lower Upper
 62 100
 64 33.6 24.2 45.0

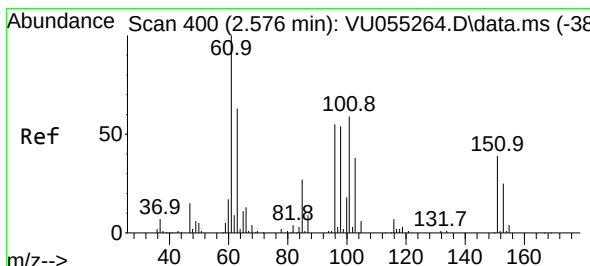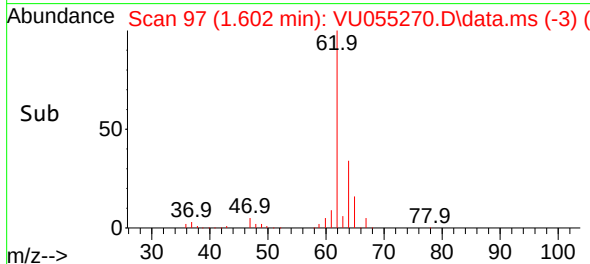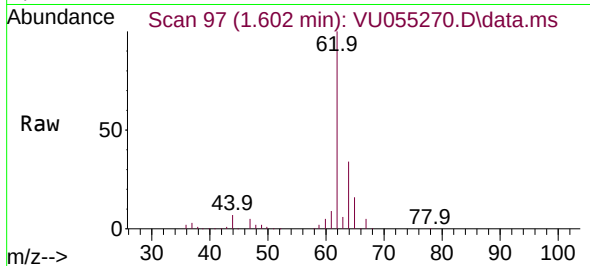

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.285 ug/L
 RT: 2.576 min Scan# 400
 Delta R.T. 0.000 min
 Lab File: VU055270.D
 Acq: 13 Sep 2023 04:15

Tgt Ion: 101 Resp: 2693
 Ion Ratio Lower Upper
 101 100
 85 47.7 37.3 55.9
 151 51.2 57.6 86.4#


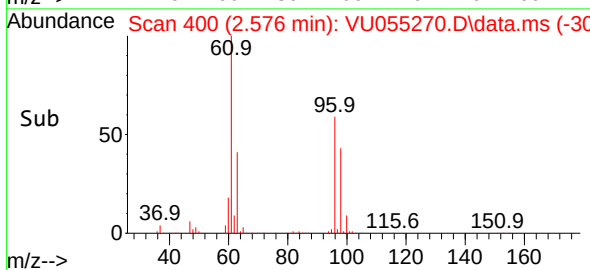

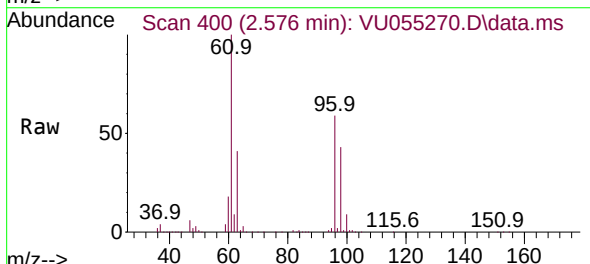


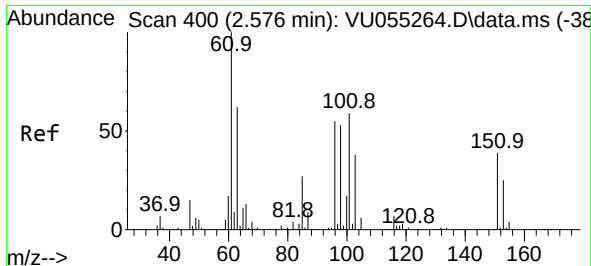

#12
1,1-Dichloroethene
Concen: 20.638 ug/L
RT: 2.576 min Scan# 400
Delta R.T. 0.000 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 96 Resp: 170646
Ion Ratio Lower Upper
96 100
61 170.4 120.8 224.4
63 69.2 94.5 175.5#

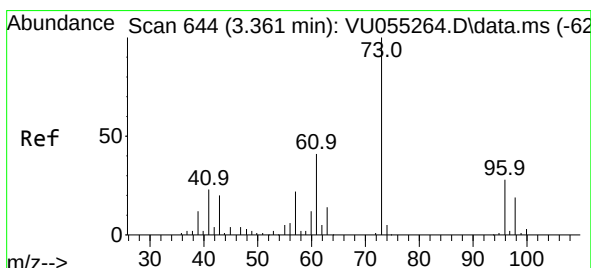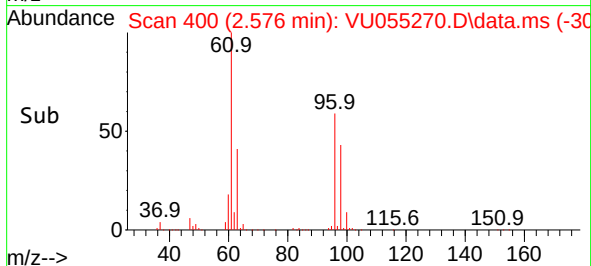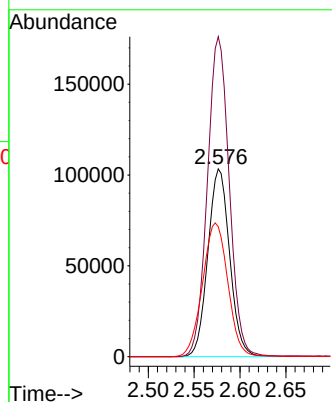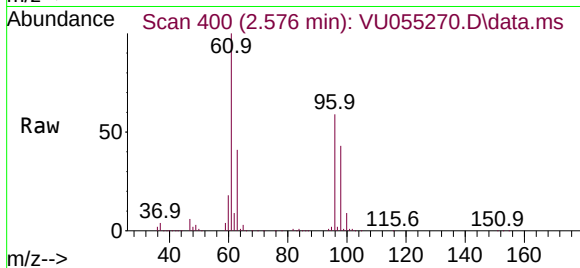

#17
Methyl tert-butyl Ether
Concen: 4.379 ug/L
RT: 3.361 min Scan# 644
Delta R.T. 0.000 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15


Tgt Ion: 73 Resp: 94966
Ion Ratio Lower Upper
73 100
43 19.1 16.2 24.2
57 21.9 17.4 26.2

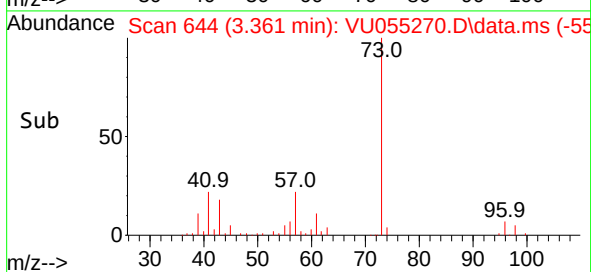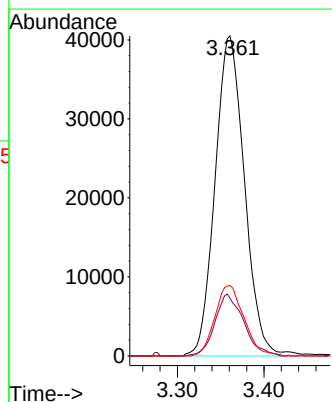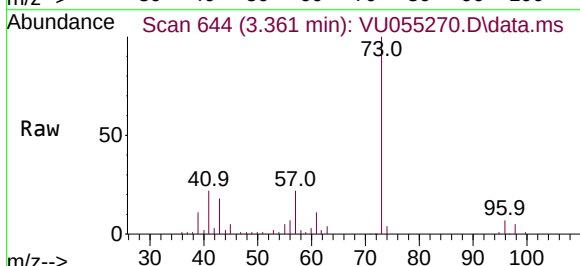



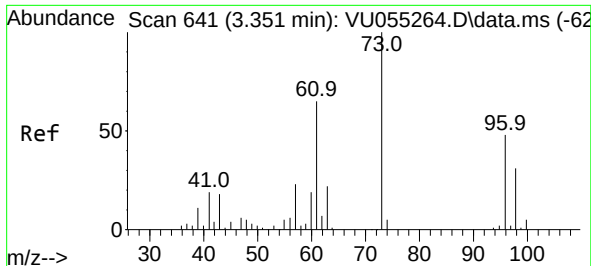


#18
trans-1,2-Dichloroethene
Concen: 0.875 ug/L
RT: 3.354 min Scan# 641
Delta R.T. 0.003 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15

Instrument :
MSVOA_U
ClientSampleId :



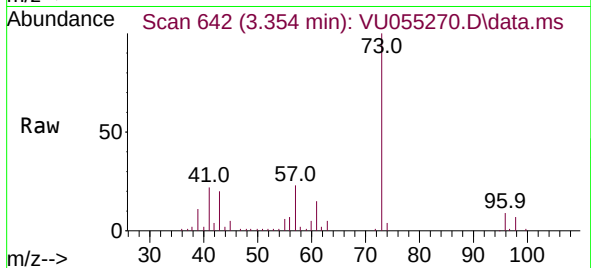



Tgt Ion: 96 Resp: 7339
Ion Ratio Lower Upper
96 100
61 153.2 108.1 200.9
98 66.9 45.4 84.4

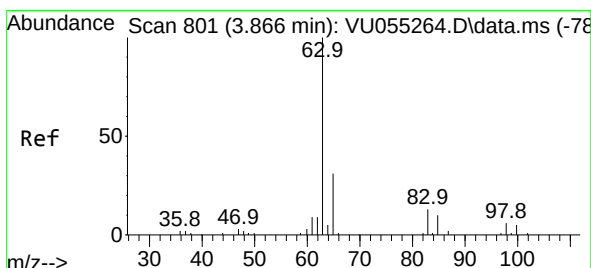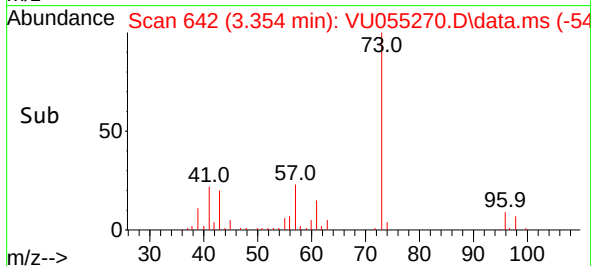

#19
1,1-Dichloroethane
Concen: 3.999 ug/L
RT: 3.866 min Scan# 801
Delta R.T. 0.000 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15

Tgt Ion: 63 Resp: 72507
Ion Ratio Lower Upper
63 100
65 33.3 22.2 41.2
83 14.0 10.6 19.8

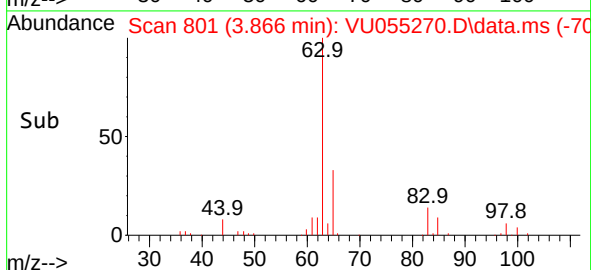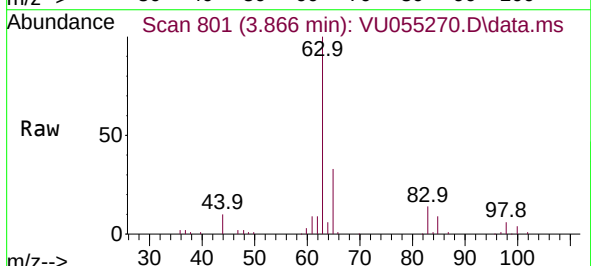




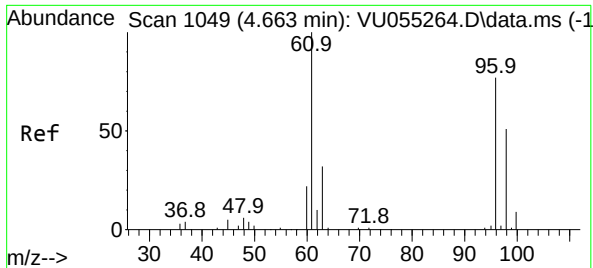


#22
 cis-1,2-Dichloroethene
 Concen: 675.786 ug/L
 RT: 4.660 min Scan# 1048
 Delta R.T. -0.003 min
 Lab File: VU055270.D
 Acq: 13 Sep 2023 04:15

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 96 Resp: 6939633




Ion	Ratio	Lower	Upper
96	100		
61	126.9	97.2	180.4
98	63.8	46.1	85.7

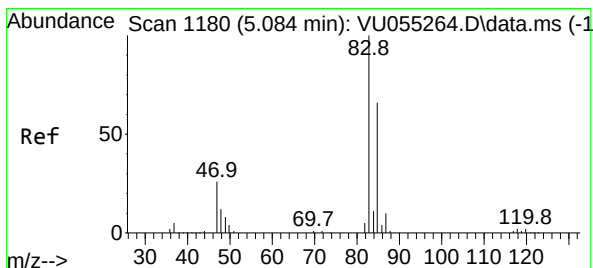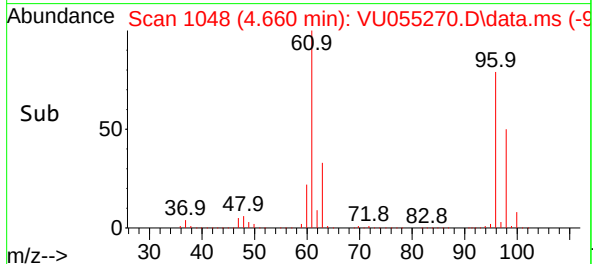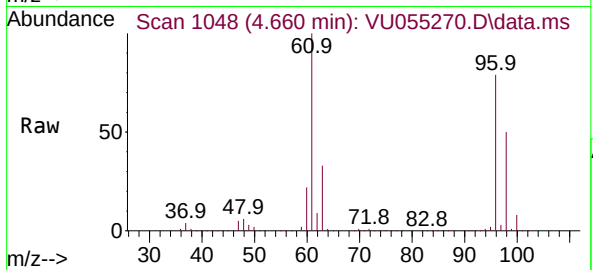


#25
 Chloroform
 Concen: 2.946 ug/L
 RT: 5.084 min Scan# 1180
 Delta R.T. 0.000 min
 Lab File: VU055270.D
 Acq: 13 Sep 2023 04:15

Tgt Ion: 83 Resp: 55633

Ion	Ratio	Lower	Upper
83	100		
85	61.1	47.2	87.6


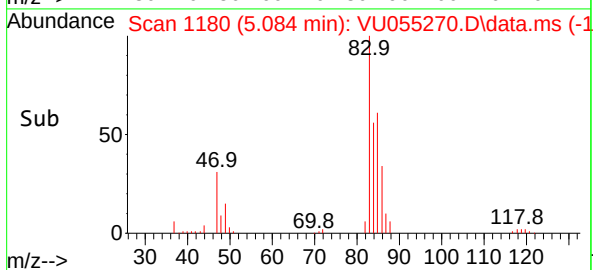

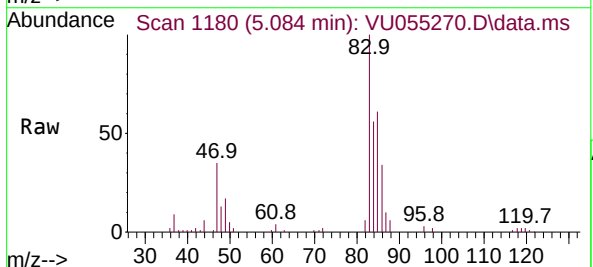


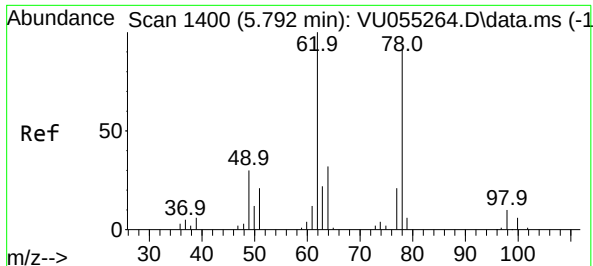

#27
1,2-Dichloroethane
Concen: 1.589 ug/L
RT: 5.795 min Scan# 1401
Delta R.T. 0.003 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 62 Resp: 18313
Ion Ratio Lower Upper
62 100
98 10.0 6.9 10.3

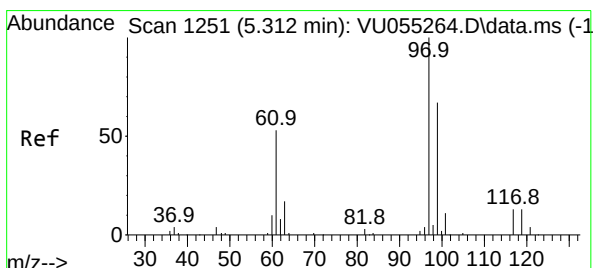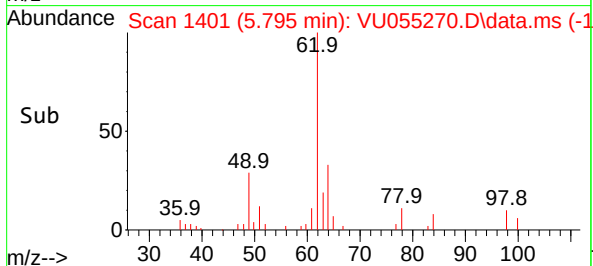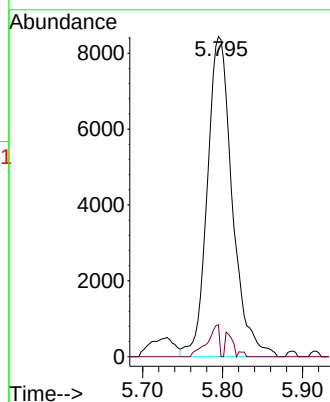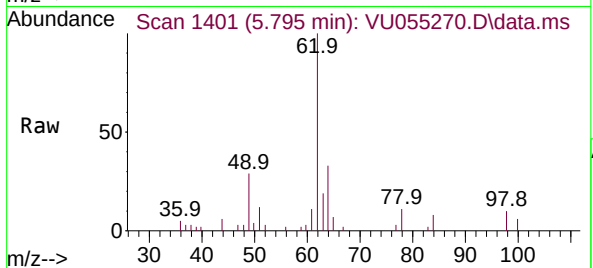

#29
1,1,1-Trichloroethane
Concen: 0.986 ug/L
RT: 5.316 min Scan# 1252
Delta R.T. 0.003 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15

Tgt Ion: 97 Resp: 16025
Ion Ratio Lower Upper
97 100
99 61.9 51.8 77.8
61 61.9 36.8 55.2#


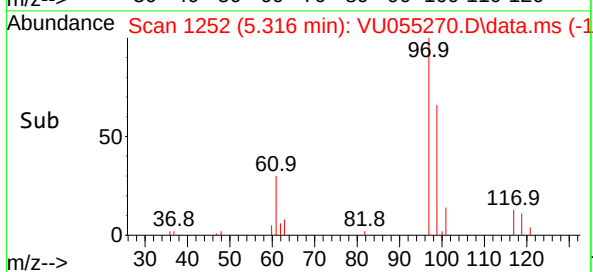
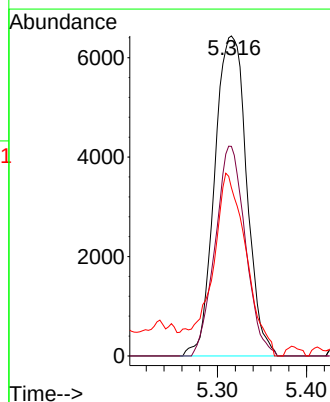
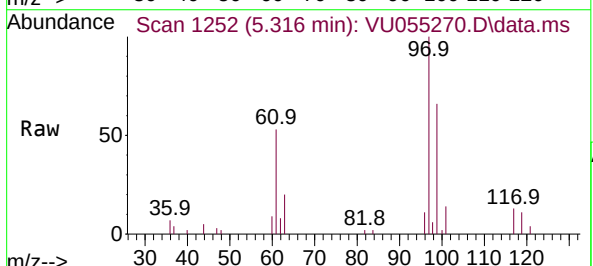


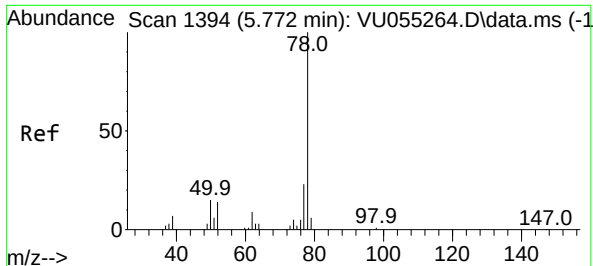

#33
Benzene
Concen: 0.146 ug/L
RT: 5.772 min Scan# 1394
Delta R.T. 0.000 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15

Instrument :
MSVOA_U
ClientSampleId :




Tgt Ion: 78 Resp: 5824

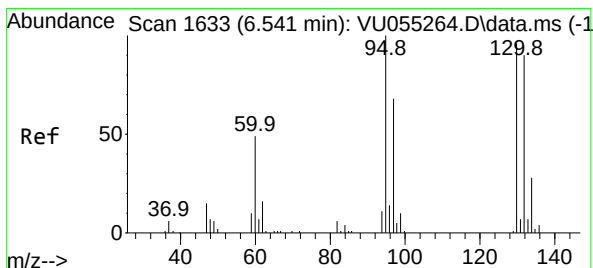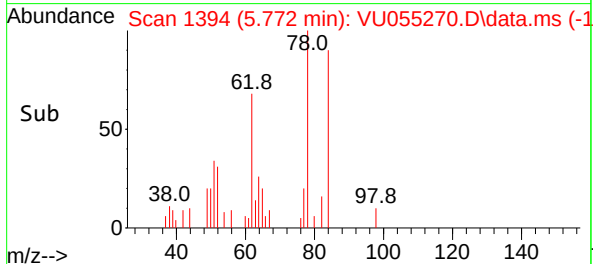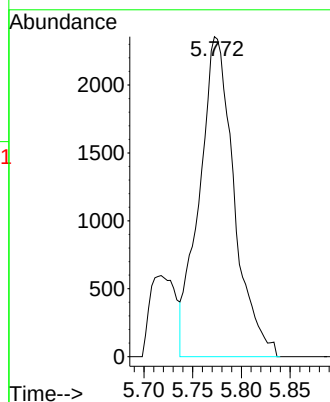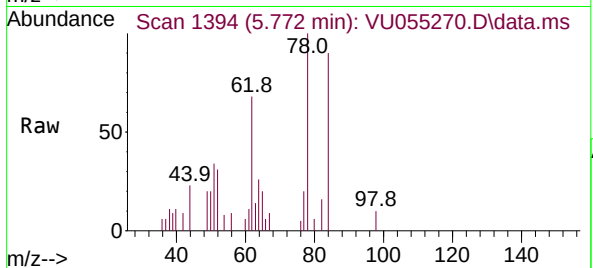


#34
Trichloroethene
Concen: 258.990 ug/L
RT: 6.541 min Scan# 1633
Delta R.T. 0.000 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15

Tgt Ion: 95 Resp: 2879494

Ion	Ratio	Lower	Upper
95	100		
97	64.1	44.7	83.1
132	89.9	66.6	123.6
130	94.1	66.5	123.5


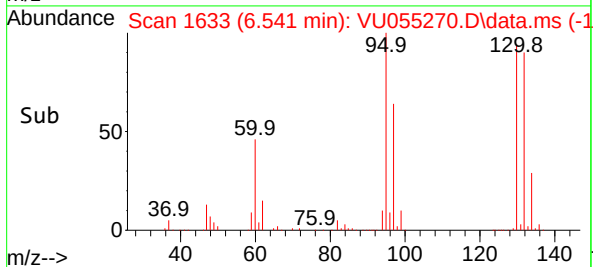

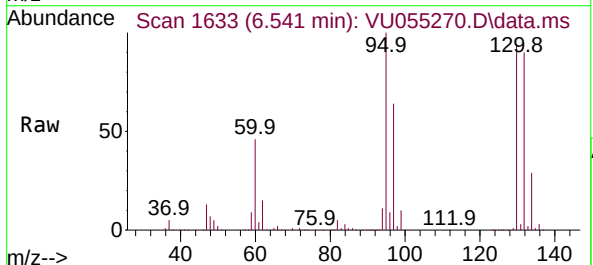


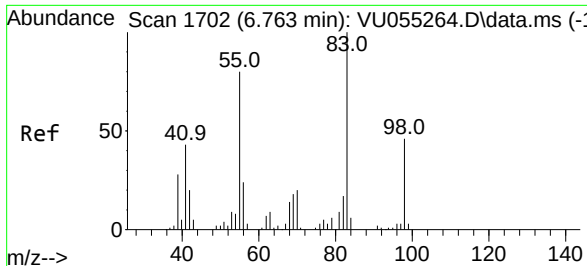

#35
Methylcyclohexane
Concen: 0.985 ug/L
RT: 6.689 min Scan# 1679
Delta R.T. -0.074 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 83 Resp: 15370
Ion Ratio Lower Upper
83 100
55 0.0 60.4 90.6#
98 62.3 35.3 52.9#

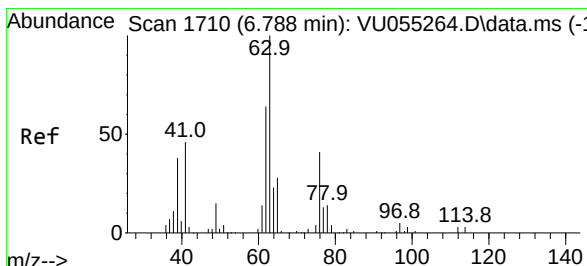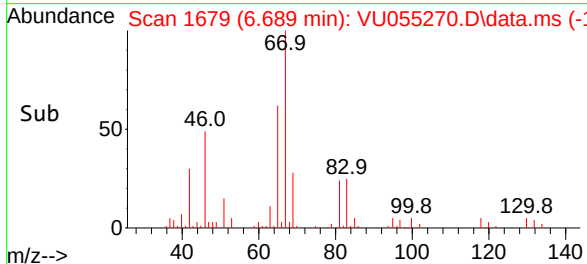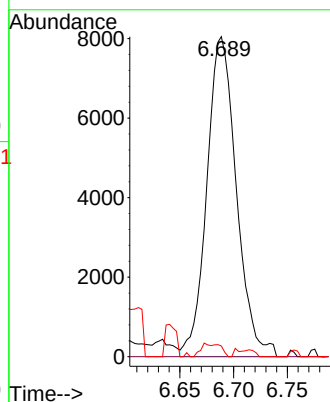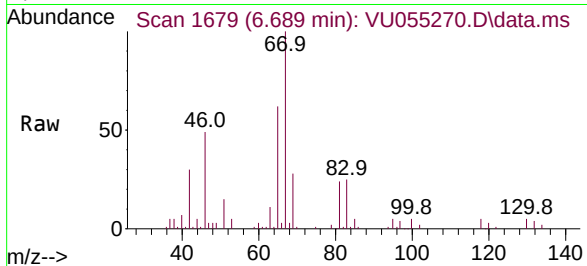

#37
1,2-Dichloropropane
Concen: 0.702 ug/L
RT: 6.685 min Scan# 1678
Delta R.T. -0.103 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15

Tgt Ion: 63 Resp: 7646
Ion Ratio Lower Upper
63 100
112 0.7 3.2 4.8#


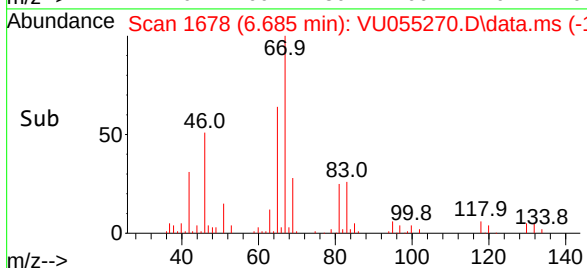

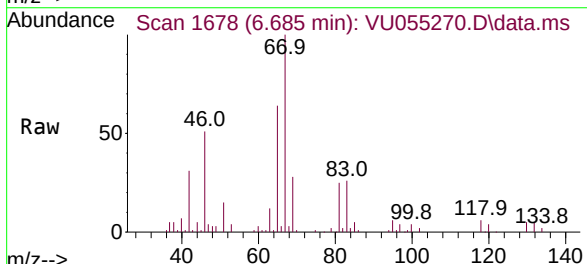


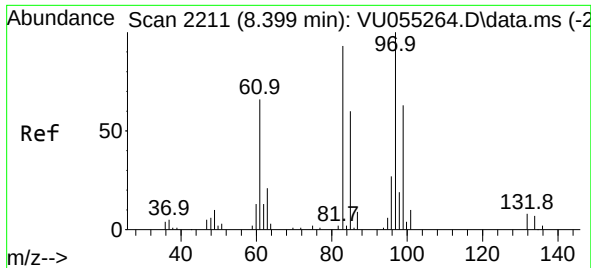

#45
1,1,2-Trichloroethane
Concen: 0.144 ug/L
RT: 8.402 min Scan# 211
Delta R.T. 0.003 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 97 Resp: 1060
Ion Ratio Lower Upper
97 100
99 0.0 44.9 83.5#
83 63.2 66.9 124.3#
85 55.4 42.2 78.4

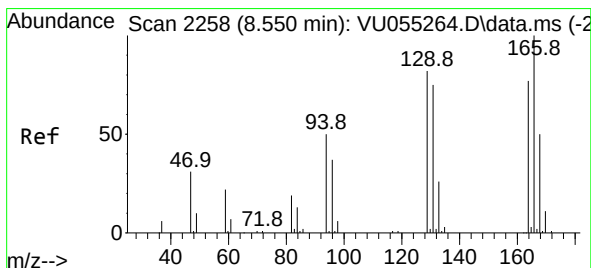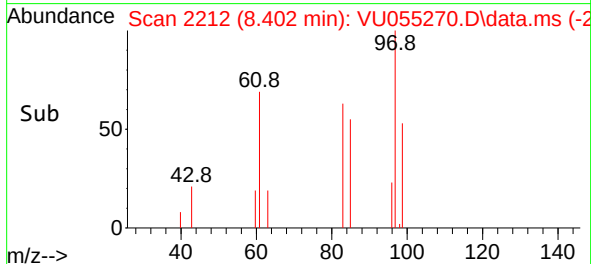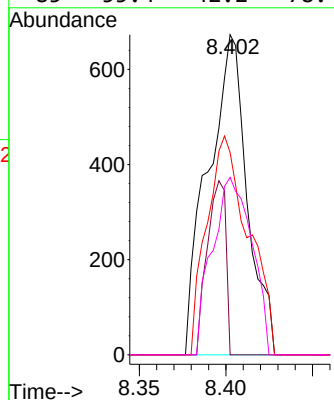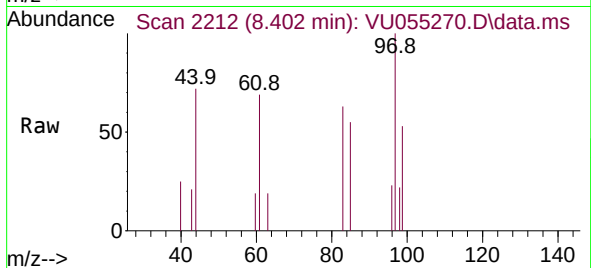

#47
Tetrachloroethene
Concen: 3.046 ug/L
RT: 8.553 min Scan# 2259
Delta R.T. 0.003 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15


Tgt Ion:164 Resp: 23409
Ion Ratio Lower Upper
164 100
129 93.5 69.2 128.6
131 89.1 68.8 127.8
166 129.6 92.3 171.5

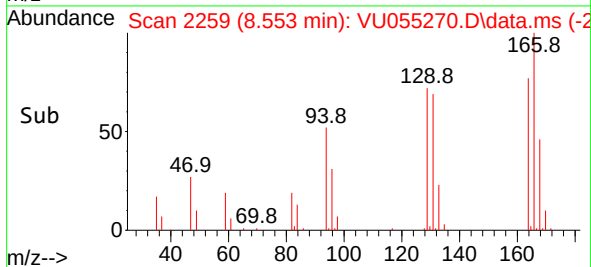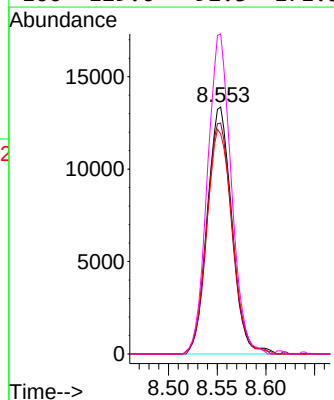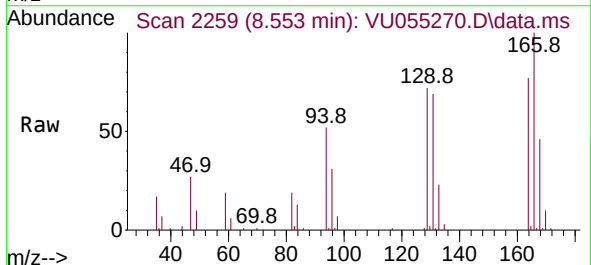



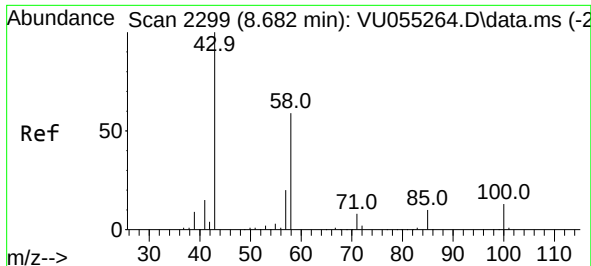


#48
2-Hexanone
Concen: 4.154 ug/L
RT: 8.679 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15

Instrument :
MSVOA_U
ClientSampleId :



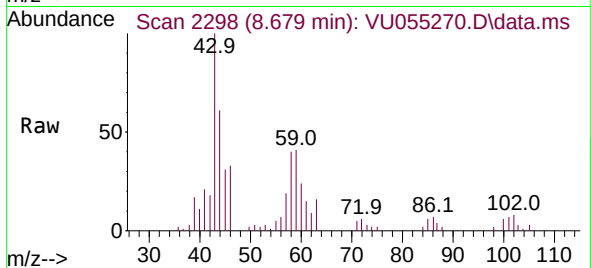



Tgt Ion: 43 Resp: 20216
Ion Ratio Lower Upper
43 100
58 43.0 44.0 66.0#
57 17.5 16.2 24.2
100 8.0 9.0 13.4#

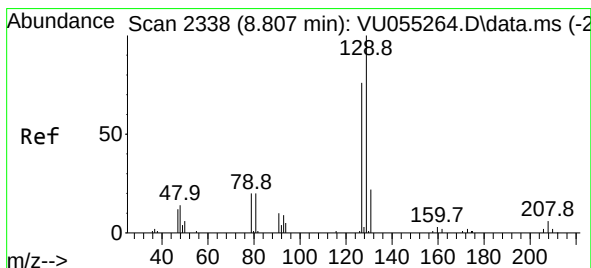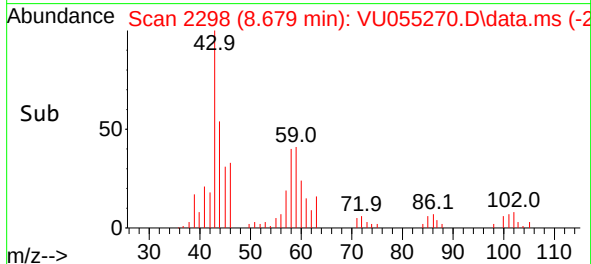

#49
Dibromochloromethane
Concen: 2.783 ug/L
RT: 8.553 min Scan# 2259
Delta R.T. -0.254 min
Lab File: VU055270.D
Acq: 13 Sep 2023 04:15


Tgt Ion:129 Resp: 22284
Ion Ratio Lower Upper
129 100
127 0.0 55.9 103.7#

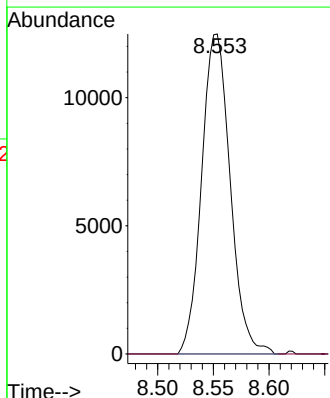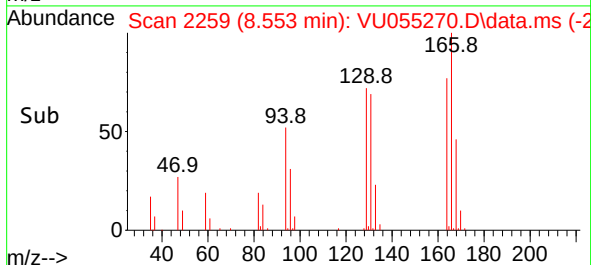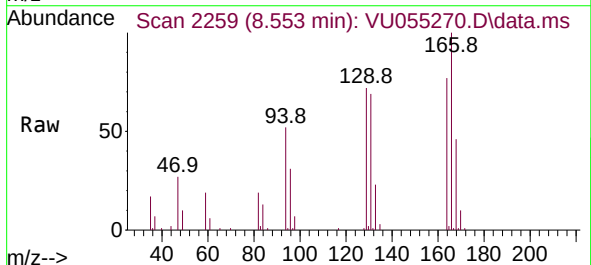

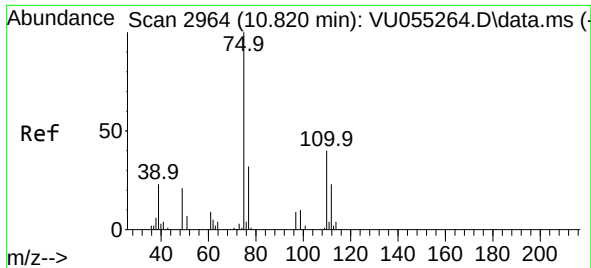

#61
 1,2,3-Trichloropropane
 Concen: 1.937 ug/L
 RT: 11.811 min Scan# 31
 Delta R.T. 0.990 min
 Lab File: VU055270.D
 Acq: 13 Sep 2023 04:15

Instrument :
 MSVOA_U
 ClientSampleId :

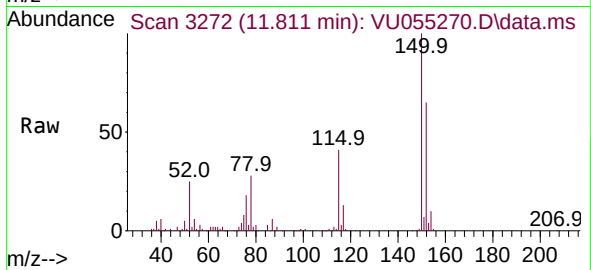

Tgt Ion:	75	Resp:	10796
Ion	Ratio	Lower	Upper
75	100		
110	2.5	28.2	42.2#
77	36.2	26.2	39.4

