

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
 Data File : VU055243.D
 Acq On : 12 Sep 2023 13:12
 Operator : MD/SY
 Sample : 04307-19DL 4X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4J2DL

Quant Time: Sep 13 01:45:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 13 01:44:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.248	114	221067	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.418	117	230026	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	107085	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	28292	2.731	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	54.600%	
7) Chloroethane-d5	1.907	69	43960	3.665	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	73.400%	
11) 1,1-Dichloroethene-d2	2.563	65	15378	2.605	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	52.000%#	
20) 2-Butanone-d5	4.624	46	112628	37.459	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	74.920%	
24) Chloroform-d	5.062	84	96691	3.517	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	70.400%	
26) 1,2-Dichloroethane-d4	5.701	65	52752	3.835	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	76.800%	
32) Benzene-d6	5.727	84	193996	3.417	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	68.400%#	
36) 1,2-Dichloropropane-d6	6.689	67	67704	3.749	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	75.000%	
41) Toluene-d8	7.898	98	162546	3.108	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	62.200%#	
43) trans-1,3-Dichloroprop...	8.184	79	14918	3.000	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	60.000%	
46) 2-Hexanone-d5	8.634	63	69932	34.636	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	69.280%	
56) 1,1,2,2-Tetrachloroeth...	10.756	84	44772	3.525	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	70.600%	
66) 1,2-Dichlorobenzene-d4	12.193	152	61006	3.903	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	78.000%#	
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.576	96	4557	0.446	ug/L	# 1
16) Methylene chloride	3.042	84	5920	0.379	ug/L	88
22) cis-1,2-Dichloroethene	4.666	96	50752	3.998	ug/L	87
34) Trichloroethene	6.541	95	58584	4.306	ug/L	97
47) Tetrachloroethene	8.553	164	4517	0.480	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055243.D
Acq On : 12 Sep 2023 13:12
Operator : MD/SY
Sample : 04307-19DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4J2DL

Quant Time: Sep 13 01:45:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 13 01:44:08 2023
Response via : Initial Calibration

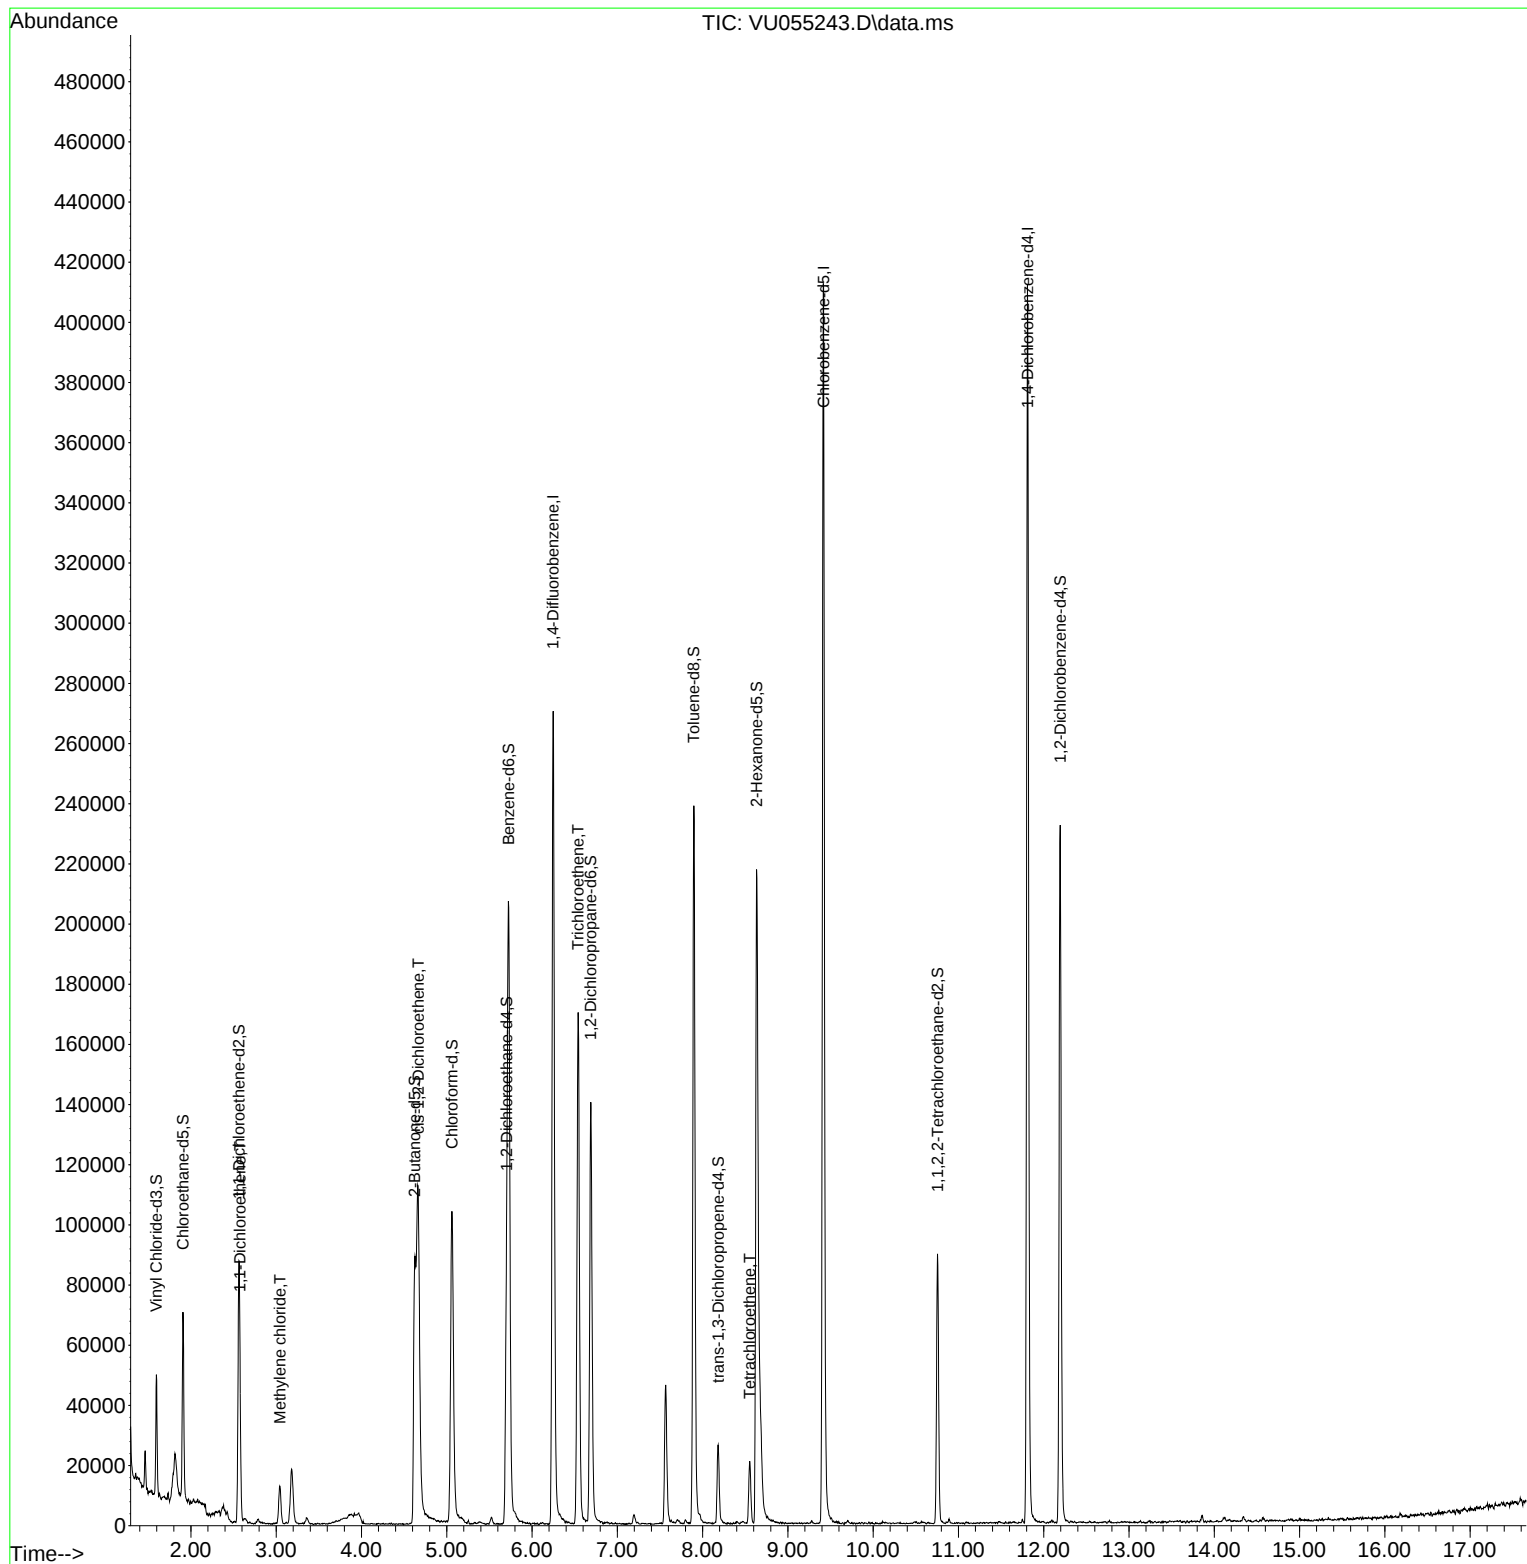

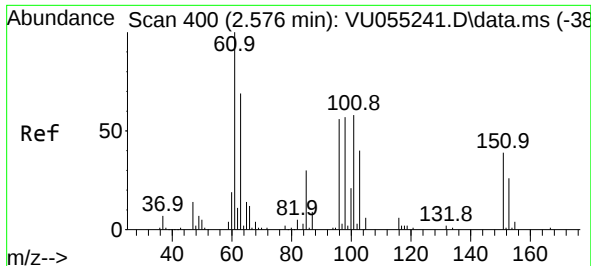

#12

1,1-Dichloroethene

Concen: 0.446 ug/L

RT: 2.576 min Scan# 400

Delta R.T. -0.000 min

Lab File: VU055243.D

Acq: 12 Sep 2023 13:12

Instrument :

MSVOA_U

ClientSampleId :

BH4J2DL





Tgt Ion: 96 Resp: 4557

Ion Ratio Lower Upper

96 100

61 235.3 120.8 224.4#

63 614.0 94.5 175.5#

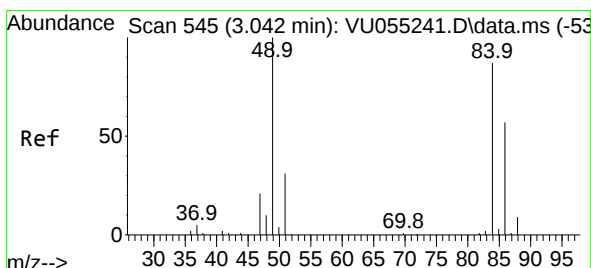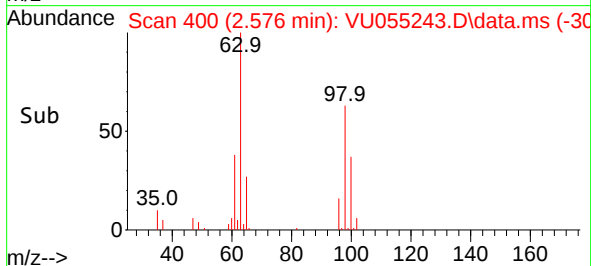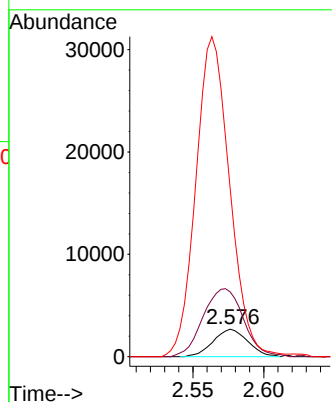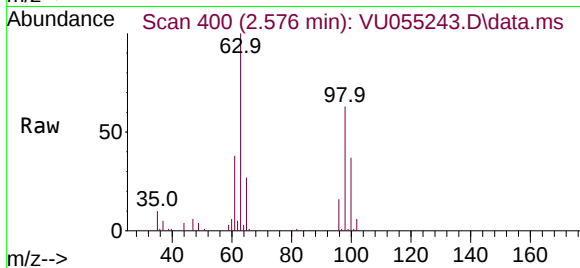

#16

Methylene chloride

Concen: 0.379 ug/L

RT: 3.042 min Scan# 545

Delta R.T. -0.000 min

Lab File: VU055243.D

Acq: 12 Sep 2023 13:12




Tgt Ion: 84 Resp: 5920


Ion Ratio Lower Upper

84 100

86 61.7 43.4 80.6

49 104.4 87.7 162.9


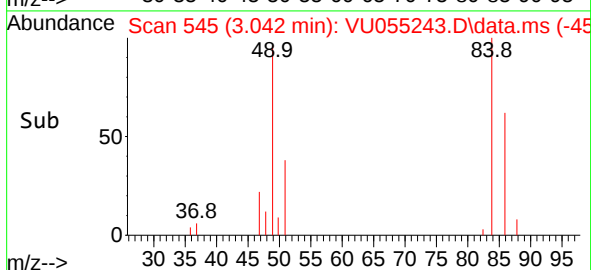
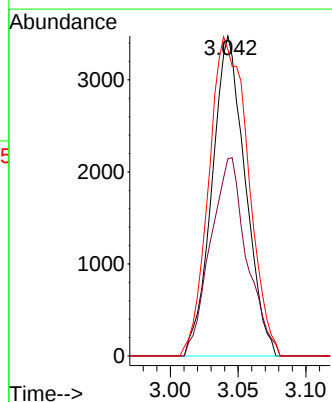
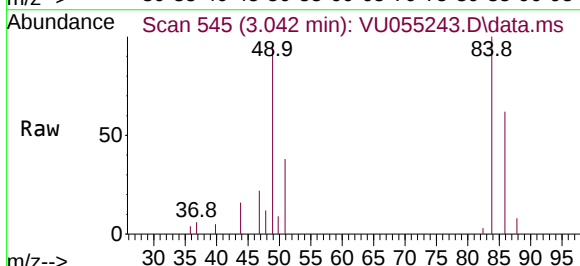


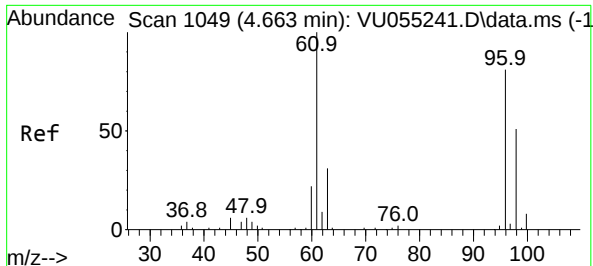

#22
cis-1,2-Dichloroethene
Concen: 3.998 ug/L
RT: 4.666 min Scan# 1050
Delta R.T. 0.003 min
Lab File: VU055243.D
Acq: 12 Sep 2023 13:12




Instrument :
MSVOA_U
ClientSampleId :
BH4J2DL


Tgt Ion: 96 Resp: 50752
Ion Ratio Lower Upper
96 100
61 121.6 97.2 180.4
98 56.9 46.1 85.7

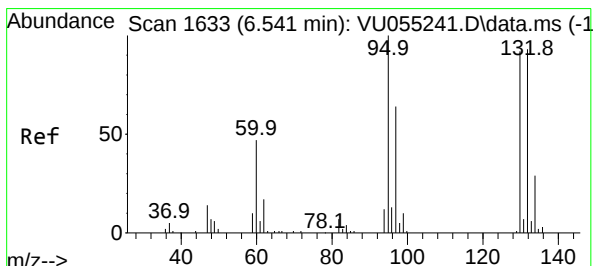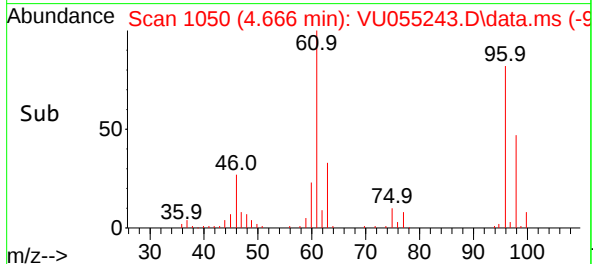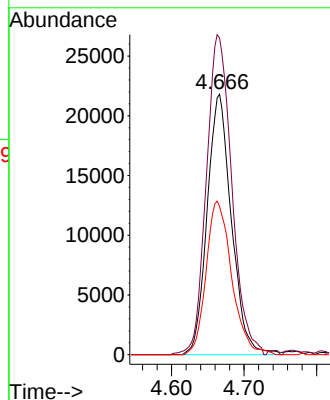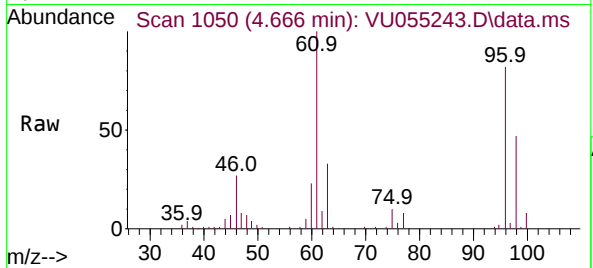

#34
Trichloroethene
Concen: 4.306 ug/L
RT: 6.541 min Scan# 1633
Delta R.T. -0.000 min
Lab File: VU055243.D
Acq: 12 Sep 2023 13:12

Tgt Ion: 95 Resp: 58584
Ion Ratio Lower Upper
95 100
97 62.9 44.7 83.1
132 92.7 66.6 123.6
130 99.5 66.5 123.5

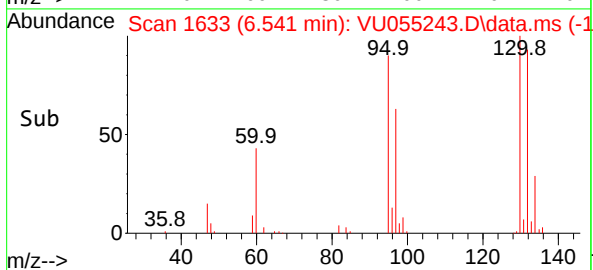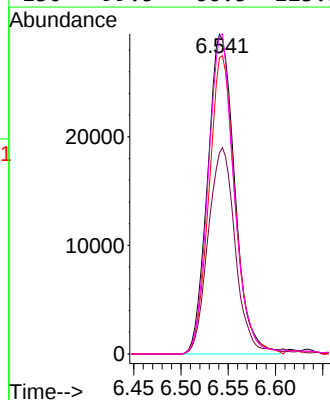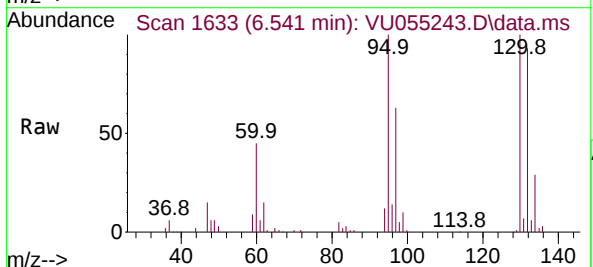

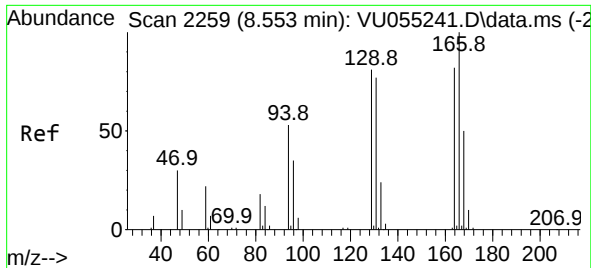

#47

Tetrachloroethene

Concen: 0.480 ug/L

RT: 8.553 min Scan# 21

Delta R.T. -0.000 min

Lab File: VU055243.D


Acq: 12 Sep 2023 13:12

Instrument :

MSVOA_U

ClientSampleId :

BH4J2DL

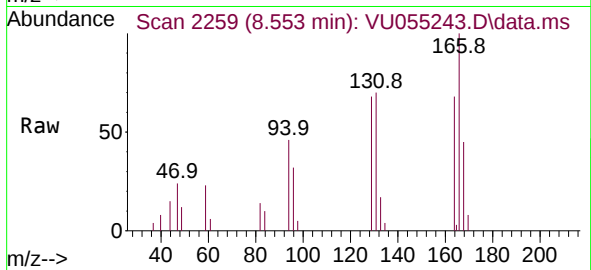

Tgt Ion:164 Resp: 4517

Ion Ratio Lower Upper

164 100

129 98.8 69.2 128.6

131 102.4 68.8 127.8

166 146.0 92.3 171.5

