

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
 Data File : VU055242.D
 Acq On : 12 Sep 2023 12:42
 Operator : MD/SY
 Sample : VU0912WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK031

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	89	95	107	rVB	44575	52405	8.13%	0.983%
2	1.904	184	191	208	rVB	104763	152478	23.66%	2.859%
3	2.563	383	396	409	rBV	91243	148244	23.00%	2.780%
4	3.042	534	545	561	rBV3	12775	24815	3.85%	0.465%
5	4.624	1028	1037	1068	rBV2	84395	234258	36.35%	4.393%
6	5.058	1157	1172	1194	rBV	120410	271014	42.05%	5.082%
7	5.724	1359	1379	1403	rBV3	224184	591020	91.70%	11.083%
8	6.245	1528	1541	1562	rBV	247424	486317	75.45%	9.119%
9	6.531	1619	1630	1645	rVB5	12751	25535	3.96%	0.479%
10	6.688	1666	1679	1704	rBV	150497	302581	46.95%	5.674%
11	7.196	1825	1837	1852	rBV5	3398	7520	1.17%	0.141%
12	7.566	1941	1952	1969	rBV2	49274	91865	14.25%	1.723%
13	7.897	2038	2055	2083	rBV	252482	456906	70.89%	8.568%
14	8.180	2134	2143	2164	rVB	28327	51113	7.93%	0.958%
15	8.634	2272	2284	2324	rBV3	252056	585485	90.84%	10.979%
16	9.415	2512	2527	2548	rBV	378486	644514	100.00%	12.086%
17	10.756	2932	2944	2960	rBV2	98566	167682	26.02%	3.144%
18	11.810	3260	3272	3290	rBV	381727	621646	96.45%	11.657%
19	12.193	3378	3391	3412	rBV	246178	410422	63.68%	7.696%
20	14.334	4049	4057	4066	rBV5	4347	6908	1.07%	0.130%




Sum of corrected areas: 5332728

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055242.D
Acq On : 12 Sep 2023 12:42
Operator : MD/SY
Sample : VU0912WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK031

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

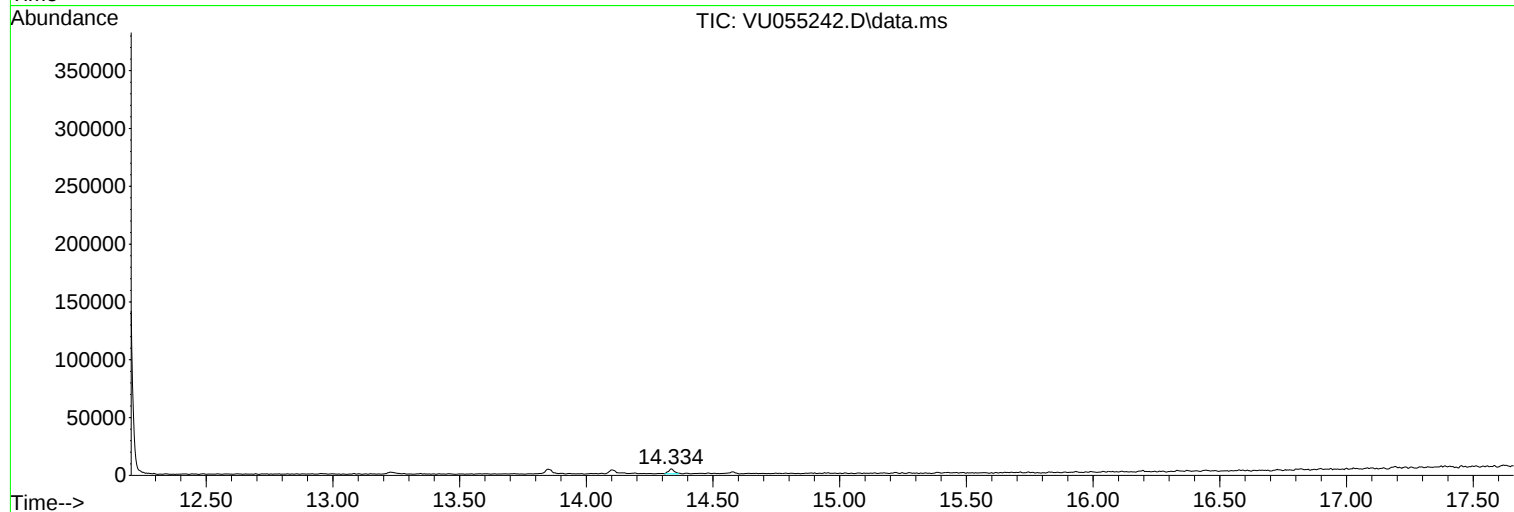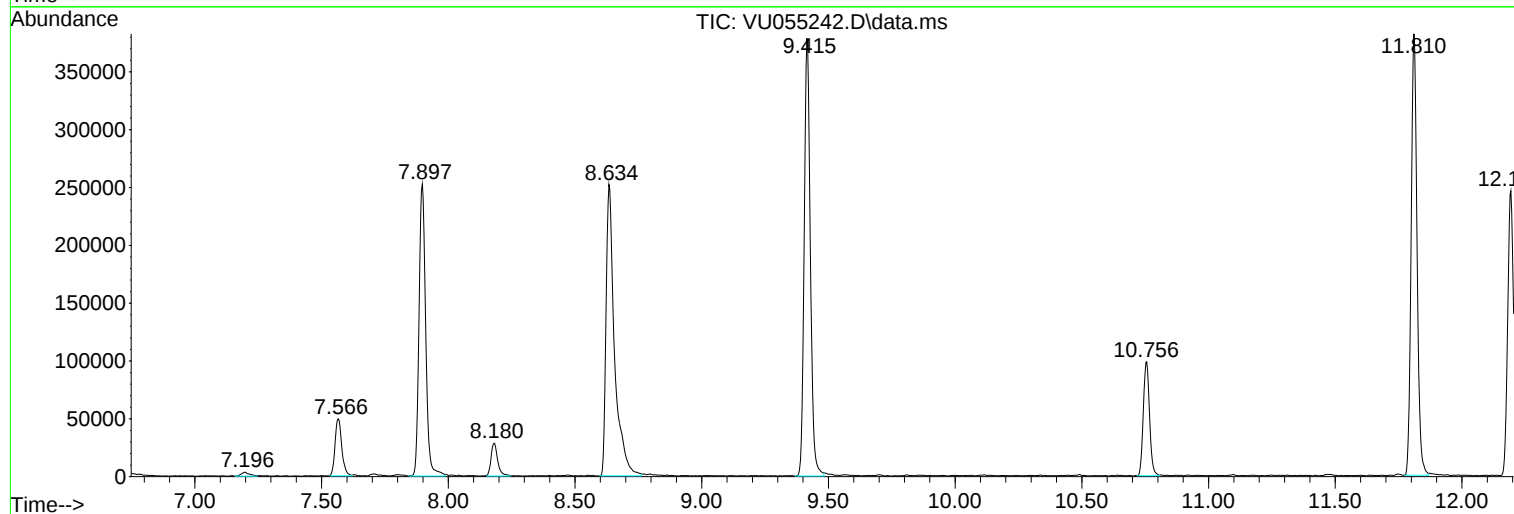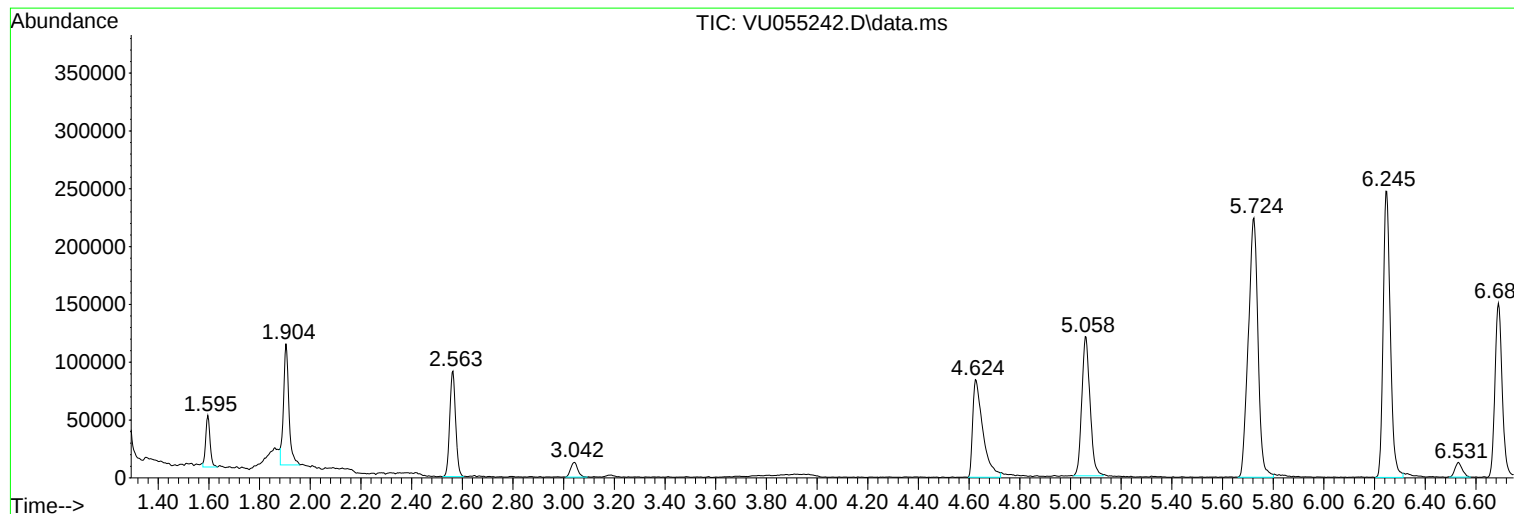

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055242.D
Acq On : 12 Sep 2023 12:42
Operator : MD/SY
Sample : VU0912WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK031

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055242.D
Acq On : 12 Sep 2023 12:42
Operator : MD/SY
Sample : VU0912WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK031

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc