

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
 Data File : VU055244.D
 Acq On : 12 Sep 2023 13:37
 Operator : MD/SY
 Sample : 04307-20DL 4X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4J3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU055244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	106	rBV	39442	46221	5.95%	0.733%
2	1.814	149	163	182	rVB4	19604	55647	7.17%	0.882%
3	1.908	184	192	205	rVB	58867	78716	10.14%	1.248%
4	2.567	383	397	412	rBV4	98177	188988	24.35%	2.997%
5	3.039	533	544	559	rBV2	13872	25212	3.25%	0.400%
6	3.178	576	587	603	rVB2	3949	9156	1.18%	0.145%
7	4.660	1023	1048	1069	rBV3	209738	661850	85.26%	10.494%
8	5.059	1157	1172	1195	rBV2	103423	246023	31.69%	3.901%
9	5.724	1357	1379	1403	rBV3	198695	537204	69.20%	8.518%
10	6.248	1529	1542	1567	rBV	250145	477253	61.48%	7.567%
11	6.541	1614	1633	1659	rBV	397157	776286	100.00%	12.309%
12	6.689	1667	1679	1697	rBV	136848	265789	34.24%	4.214%
13	7.566	1938	1952	1967	rBV2	44983	81700	10.52%	1.295%
14	7.898	2039	2055	2075	rBV	234444	412939	53.19%	6.548%
15	8.181	2130	2143	2163	rBV4	24326	45549	5.87%	0.722%
16	8.554	2249	2259	2272	rVB3	33900	58005	7.47%	0.920%
17	8.634	2272	2284	2316	rBV3	225241	525141	67.65%	8.327%
18	9.415	2514	2527	2554	rBV	383321	649384	83.65%	10.297%
19	10.756	2932	2944	2962	rBV	89922	151023	19.45%	2.395%
20	11.811	3258	3272	3293	rBV	391747	636080	81.94%	10.086%
21	12.193	3377	3391	3410	rBV2	221688	378615	48.77%	6.003%




Sum of corrected areas: 6306781

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055244.D
Acq On : 12 Sep 2023 13:37
Operator : MD/SY
Sample : 04307-20DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4J3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

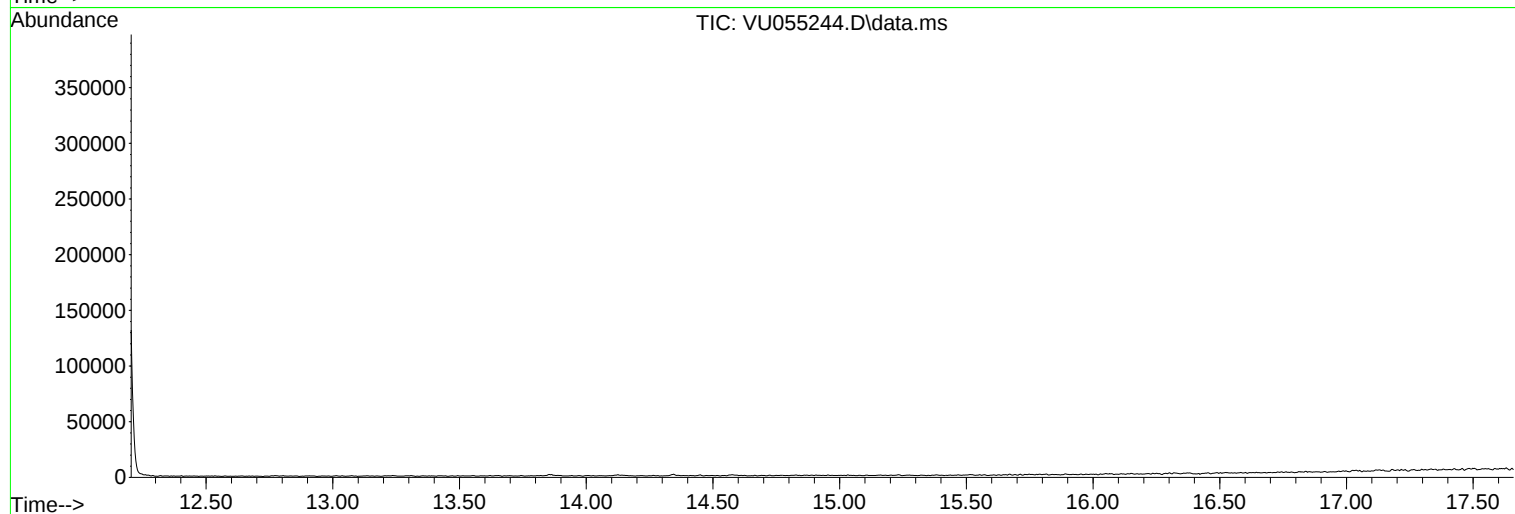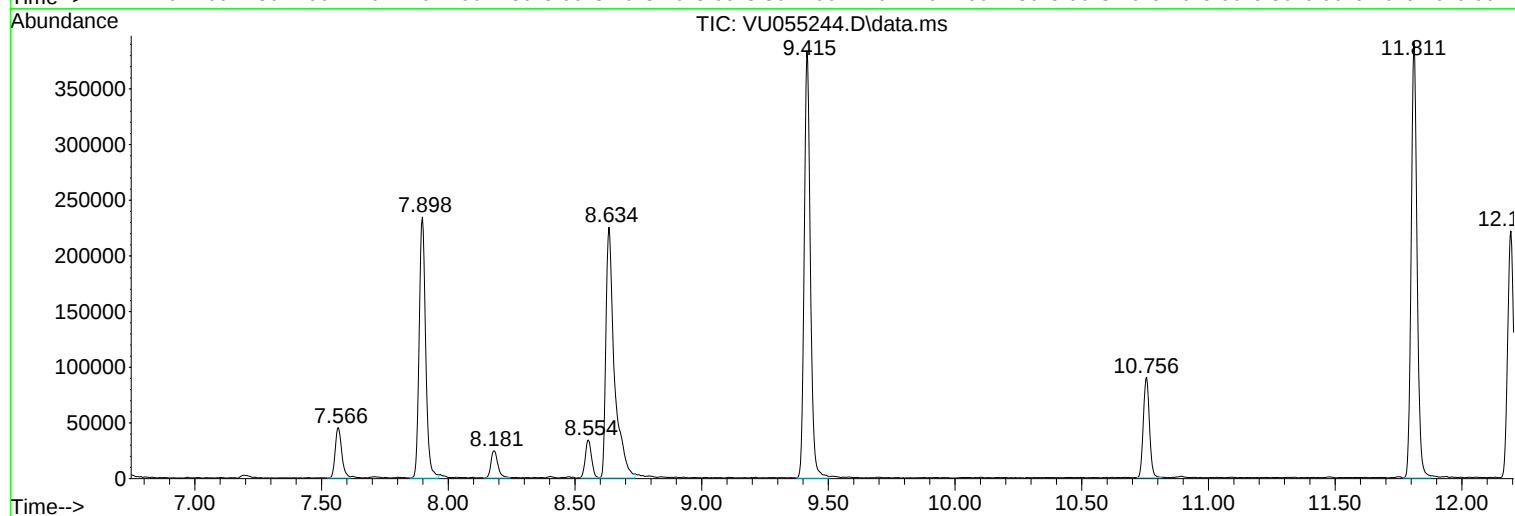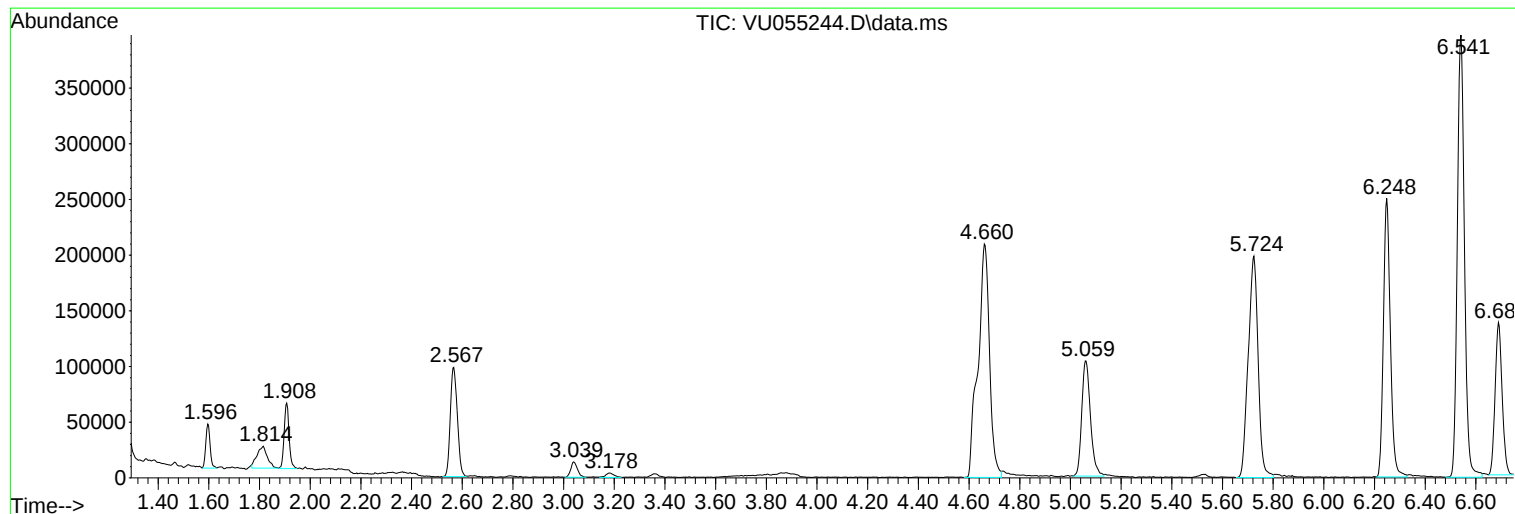

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055244.D
Acq On : 12 Sep 2023 13:37
Operator : MD/SY
Sample : 04307-20DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4J3DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.814	0.58 ug/L	55647	1,4-Difluorobenzene	6.248

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			N-(3,5-Dinitropyridin-2-yl)-L-as...	300	C9H8N4O8	035899-60-6	17
2			Benzeneethanamine, 2-fluoro-.bet...	185	C9H12FN02	103439-04-9	17
3			3-Cyclohexyl-1-methyl-1-(2-pheny...	260	C16H24N2O	1024470-80-1	12
4			Ethylamine, 2-(adamantan-1-yl)-1...	193	C13H23N	1000310-59-0	12
5			(R)-(-)-2-Amino-1-propanol	75	C3H9NO	035320-23-1	9

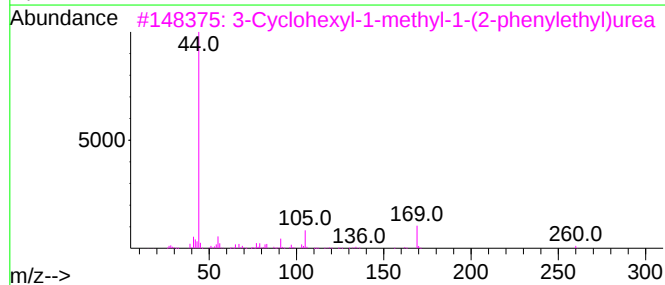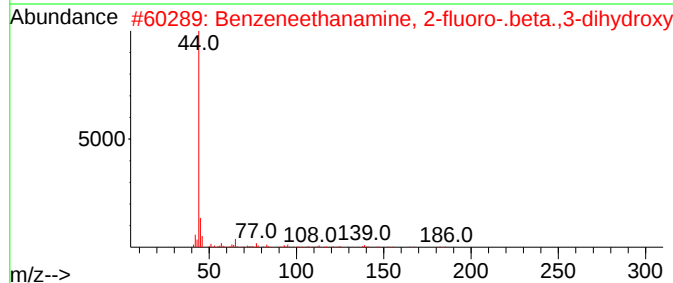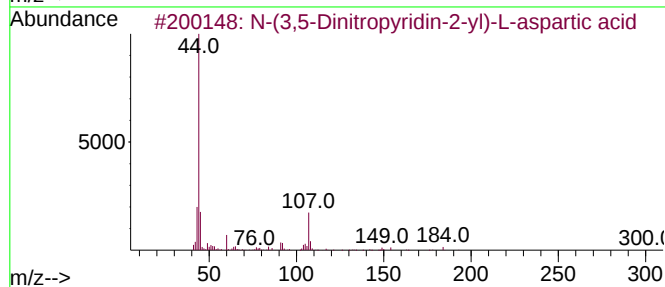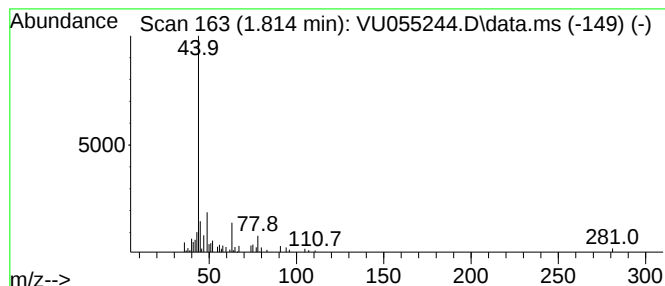

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055244.D
Acq On : 12 Sep 2023 13:37
Operator : MD/SY
Sample : 04307-20DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4J3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.814	0.6	ug/L	55647	1	6.248	477253	5.0