

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
 Data File : VU055260.D
 Acq On : 12 Sep 2023 20:08
 Operator : MD/SY
 Sample : VIBLK130
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK130

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055260.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	109	rVB	47657	57587	8.71%	1.113%
2	1.821	157	165	168	rBV5	6938	10542	1.60%	0.204%
3	1.904	184	191	207	rVB	71825	99794	15.10%	1.929%
4	2.564	384	396	412	rBV	92782	152665	23.10%	2.950%
5	3.043	533	545	561	rVB	12538	23982	3.63%	0.463%
6	3.181	576	588	608	rVB	12152	27266	4.13%	0.527%
7	4.625	1025	1037	1066	rBV2	100950	273396	41.37%	5.283%
8	5.062	1157	1173	1196	rBV2	113333	260810	39.46%	5.040%
9	5.724	1358	1379	1404	rBV2	214594	565647	85.59%	10.931%
10	6.248	1529	1542	1561	rBV	213188	402829	60.95%	7.785%
11	6.531	1615	1630	1647	rBV8	14980	32764	4.96%	0.633%
12	6.689	1666	1679	1696	rBV2	145645	286893	43.41%	5.544%
13	7.567	1941	1952	1967	rBV	46859	83789	12.68%	1.619%
14	7.898	2039	2055	2077	rBV	256687	450940	68.23%	8.714%
15	8.181	2131	2143	2160	rBV	28126	50504	7.64%	0.976%
16	8.634	2273	2284	2319	rBV3	281368	660912	100.00%	12.772%
17	9.415	2515	2527	2552	rBV	337483	576097	87.17%	11.133%
18	10.756	2932	2944	2957	rBV	108698	173609	26.27%	3.355%
19	11.811	3260	3272	3294	rBV	347349	566219	85.67%	10.942%
20	12.193	3379	3391	3409	rBV	249348	418353	63.30%	8.085%




Sum of corrected areas: 5174598

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055260.D
Acq On : 12 Sep 2023 20:08
Operator : MD/SY
Sample : VIBLK130
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

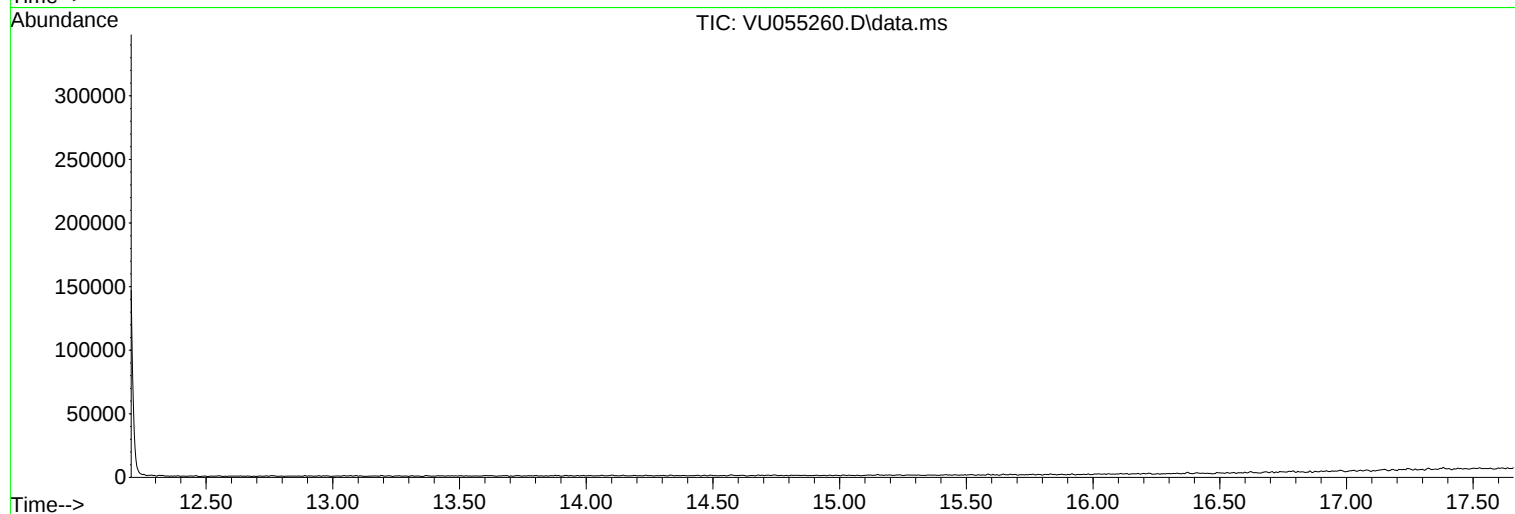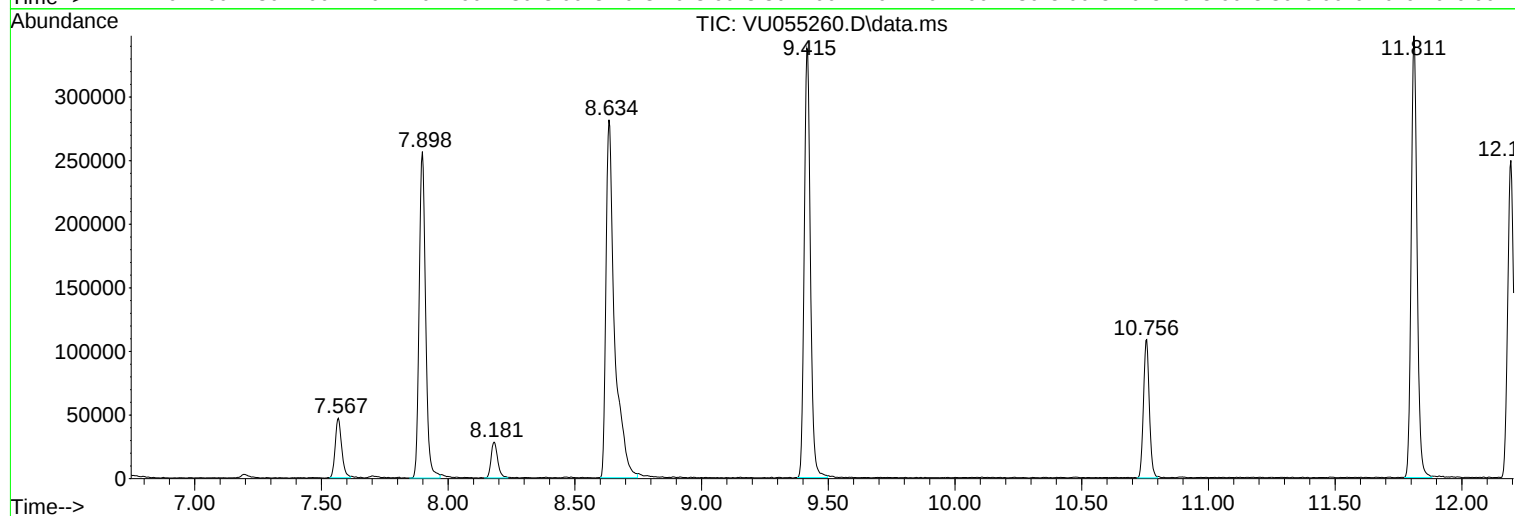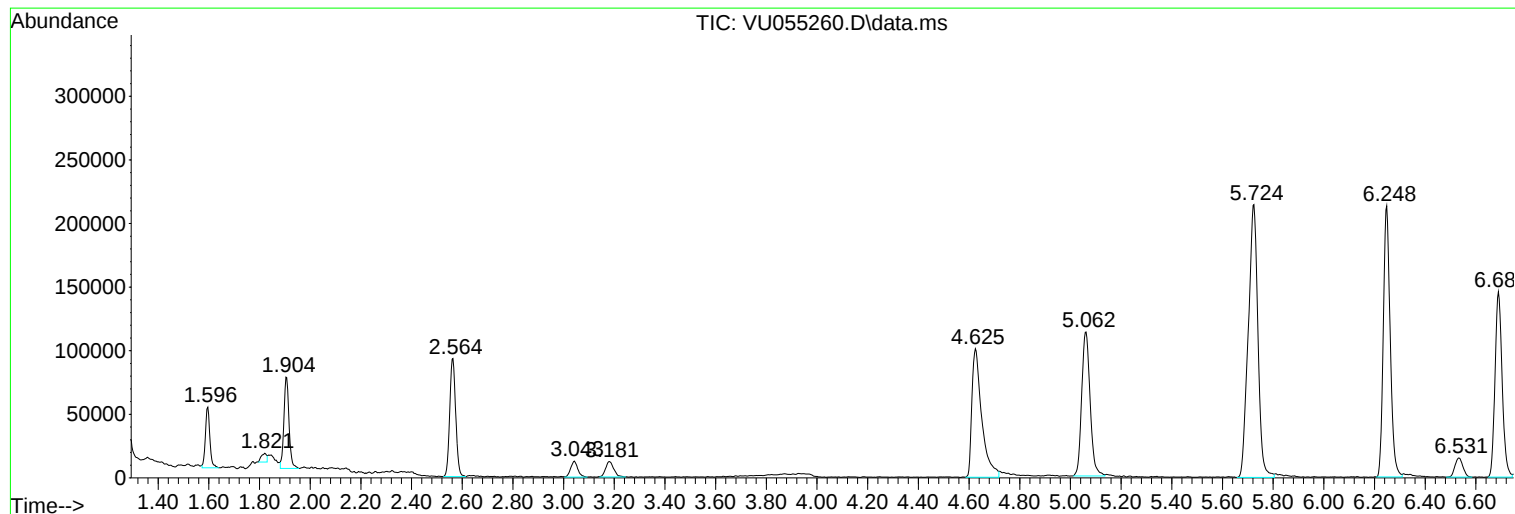

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055260.D
Acq On : 12 Sep 2023 20:08
Operator : MD/SY
Sample : VIBLK130
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055260.D
Acq On : 12 Sep 2023 20:08
Operator : MD/SY
Sample : VIBLK130
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc