

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
 Data File : VU055266.D
 Acq On : 13 Sep 2023 02:37
 Operator : MD/SY
 Sample : 04350-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4M8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055266.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.470	51	56	65	rVB3	10303	10970	1.54%	0.187%
2	1.602	87	97	114	rVB	600625	710665	100.00%	12.090%
3	1.907	185	192	204	rVB	55955	70736	9.95%	1.203%
4	2.563	379	396	411	rBV2	81589	135905	19.12%	2.312%
5	3.357	633	643	662	rVB4	16304	37040	5.21%	0.630%
6	4.663	1027	1049	1071	rBV3	190389	620260	87.28%	10.552%
7	5.062	1157	1173	1194	rBV2	102877	238053	33.50%	4.050%
8	5.724	1360	1379	1406	rBV2	188179	502274	70.68%	8.545%
9	6.248	1528	1542	1564	rBV	216929	422337	59.43%	7.185%
10	6.541	1619	1633	1652	rBV5	70448	139671	19.65%	2.376%
11	6.689	1666	1679	1707	rBV	126402	257776	36.27%	4.385%
12	7.566	1940	1952	1970	rBV2	39724	72523	10.20%	1.234%
13	7.897	2041	2055	2070	rBV	215123	379725	53.43%	6.460%
14	7.971	2070	2078	2092	rVB	13704	27372	3.85%	0.466%
15	8.184	2132	2144	2161	rBV2	22360	39468	5.55%	0.671%
16	8.637	2272	2285	2316	rBV4	215515	532078	74.87%	9.052%
17	9.418	2516	2528	2548	rBV	341386	592871	83.42%	10.086%
18	10.756	2932	2944	2960	rBV	87989	146155	20.57%	2.486%
19	11.810	3260	3272	3293	rBV	348004	569317	80.11%	9.685%
20	12.074	3343	3354	3365	rBV5	8012	20044	2.82%	0.341%
21	12.193	3379	3391	3410	rBV	213487	352989	49.67%	6.005%




Sum of corrected areas: 5878229

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055266.D
Acq On : 13 Sep 2023 02:37
Operator : MD/SY
Sample : 04350-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

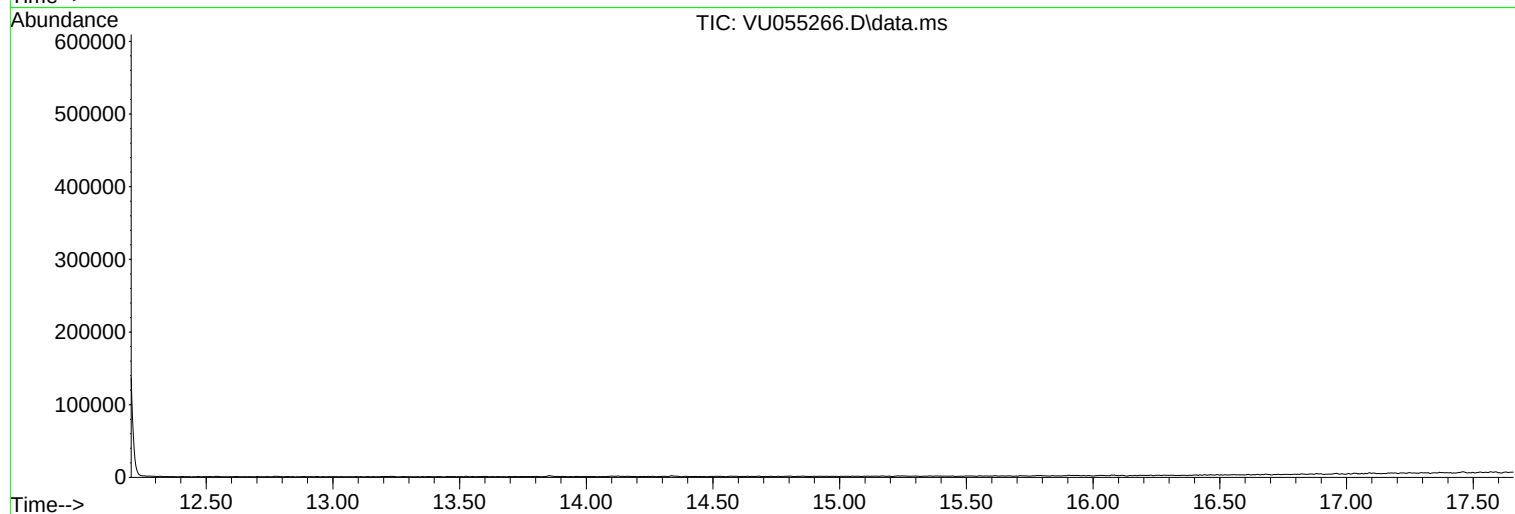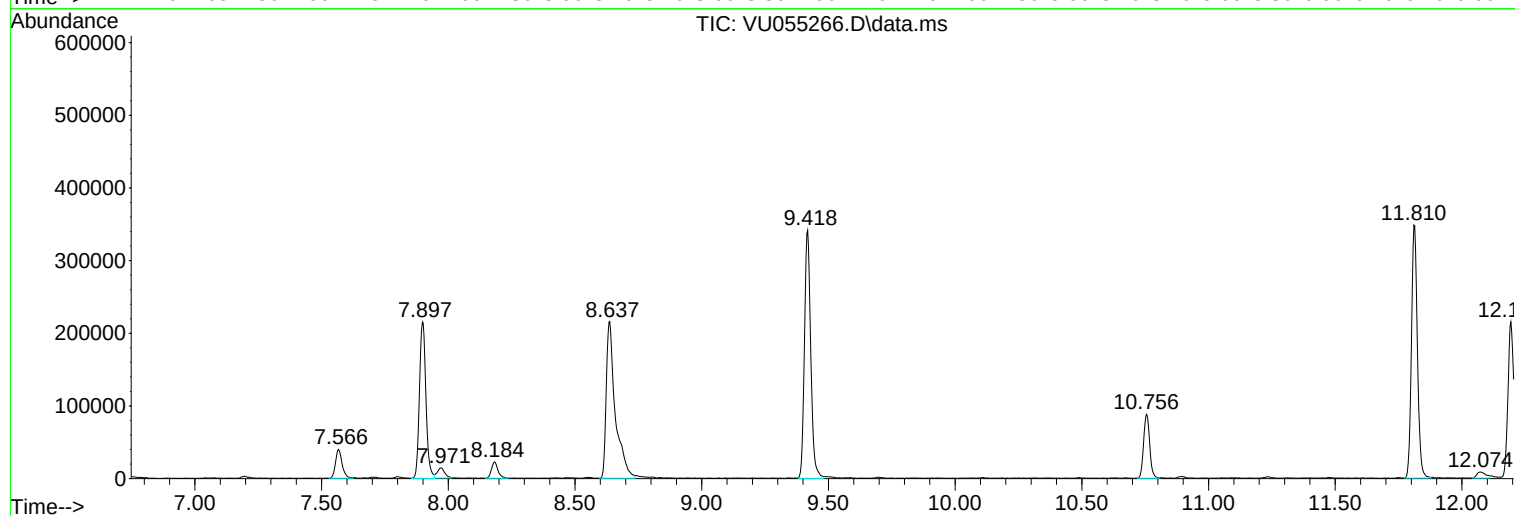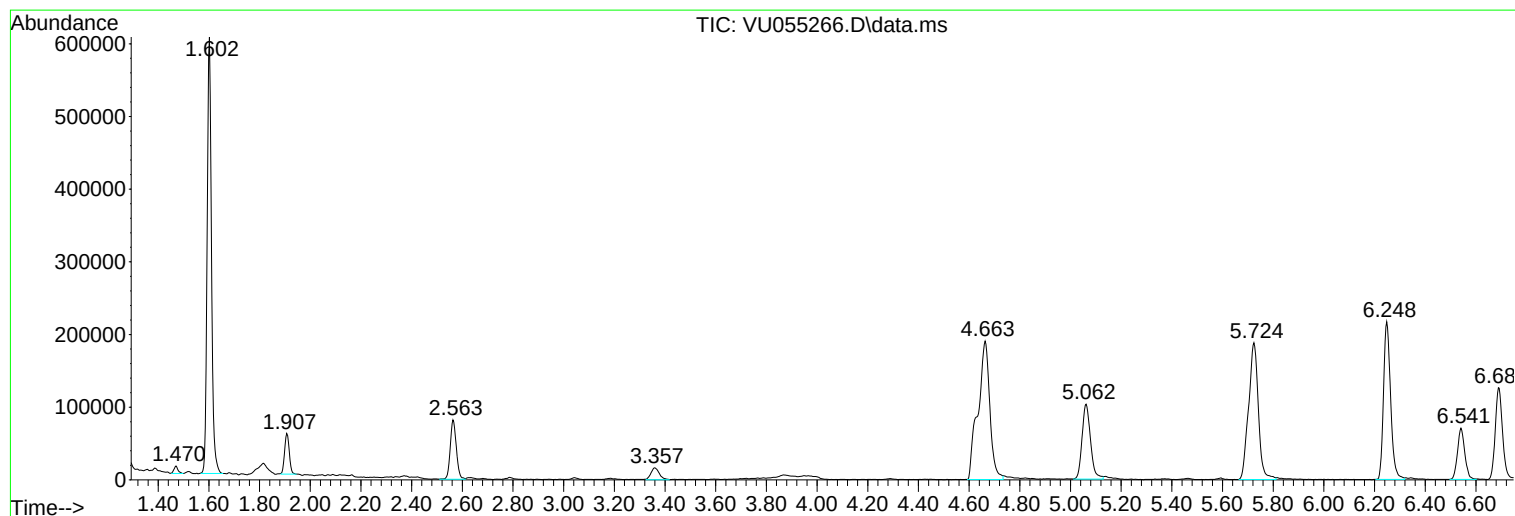

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055266.D
Acq On : 13 Sep 2023 02:37
Operator : MD/SY
Sample : 04350-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
Data File : VU055266.D
Acq On : 13 Sep 2023 02:37
Operator : MD/SY
Sample : 04350-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc