
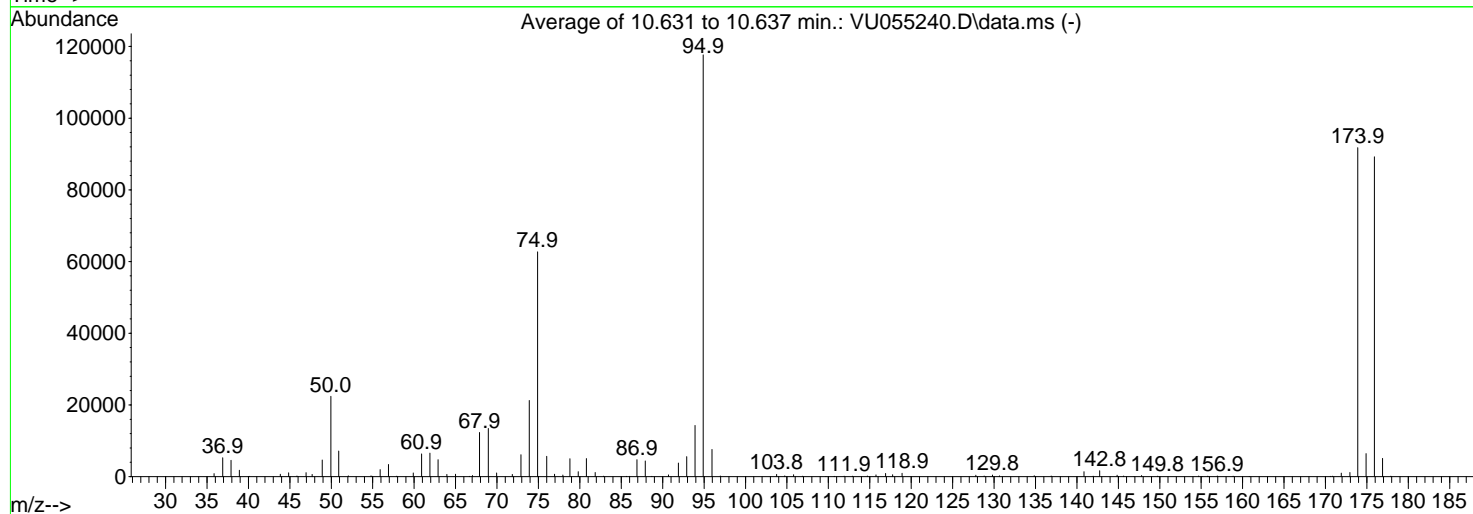


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091223\
 Data File : VU055240.D
 Acq On : 12 Sep 2023 10:12
 Operator : MD/SY
 Sample : BFB042
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB042

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Sep 15 02:53:52 2023

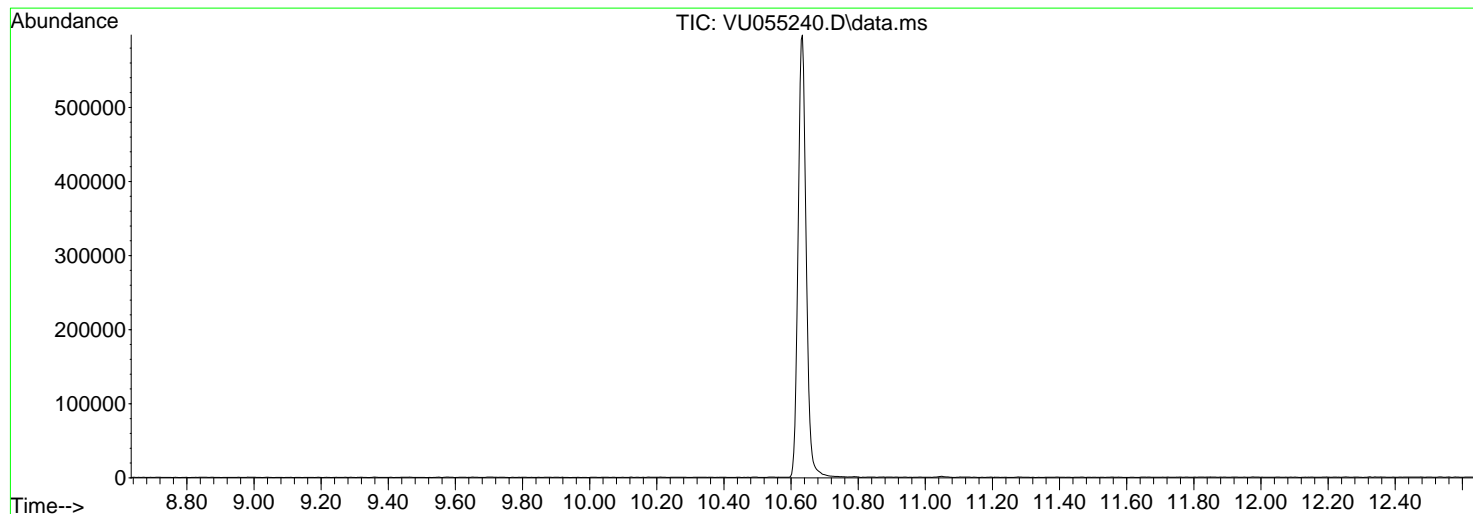

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	22395	PASS
75	95	30	80	53.3	62709	PASS
95	95	100	100	100.0	117664	PASS
96	95	5	9	6.5	7592	PASS
173	174	0.00	2	1.3	1159	PASS
174	95	50	120	78.0	91771	PASS
175	174	5	9	7.0	6424	PASS
176	174	95	101	97.2	89205	PASS
177	176	5	9	5.7	5070	PASS

m/z	Abundance
39.80	189.0
43.90	656.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.80	706.0
36.90	5566.0
37.90	4585.0
38.90	1837.0
40.10	169.0
43.80	1259.0
44.80	1101.0
45.90	184.0
46.90	1097.0
47.70	748.0
48.90	4924.0
49.90	23872.0
50.90	7515.0
52.00	252.0
54.80	358.0
55.90	1936.0
56.90	3678.0
57.90	142.0
59.90	959.0
60.90	6560.0
61.90	6805.0
62.90	4722.0
63.90	638.0
65.00	760.0
66.70	270.0
67.00	274.0
67.90	12870.0
68.90	13430.0
69.90	1001.0
71.80	723.0
72.90	6262.0
73.90	21944.0
74.90	64528.0
76.00	5915.0
77.00	606.0
77.90	557.0
78.80	5080.0
79.80	1437.0
80.80	5154.0
81.90	1168.0
82.90	114.0
85.70	102.0
86.90	4740.0
87.90	4568.0
90.70	556.0
91.90	4135.0
92.90	5736.0
93.90	14672.0
94.90	120856.0
95.90	8054.0
97.00	213.0
103.70	768.0
104.70	204.0
105.80	523.0
106.90	133.0
109.70	100.0
110.70	113.0
111.90	133.0
112.80	161.0
114.70	167.0
115.70	446.0
116.90	937.0
117.80	570.0
118.90	984.0
127.80	468.0
128.80	166.0
129.80	459.0
130.60	194.0
134.90	297.0
136.90	182.0
140.90	1393.0
141.90	144.0
142.70	1497.0
144.90	316.0
145.70	182.0
146.90	105.0
147.80	348.0
149.80	122.0
154.70	198.0
155.80	124.0
156.90	183.0
158.80	137.0
170.90	242.0
171.90	918.0
173.00	1095.0
173.90	91320.0
174.90	6734.0
175.90	88848.0
176.90	4982.0
177.90	199.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	868.0
36.90	5433.0
37.90	4626.0
38.90	1804.0
39.80	129.0
40.10	136.0
43.80	1301.0
44.80	1055.0
45.80	201.0
46.90	1080.0
47.70	644.0
48.90	4914.0
50.00	23016.0
50.90	7375.0
52.10	221.0
54.80	356.0
55.90	1999.0
56.90	3459.0
57.90	154.0
59.90	1089.0
60.90	6585.0
61.90	6851.0
62.90	4828.0
63.90	640.0
65.00	729.0
67.10	321.0
67.90	12562.0
69.00	13935.0
70.00	1054.0
71.90	627.0
72.90	6318.0
73.90	21856.0
74.90	64112.0
76.00	5786.0
76.90	677.0
77.90	464.0
78.80	5229.0
79.80	1486.0
80.80	5193.0
81.80	1199.0
82.80	125.0
85.70	117.0
86.00	108.0
86.90	4853.0
87.90	4422.0
88.70	142.0
90.70	500.0
91.90	3896.0
92.90	5760.0
93.90	14719.0
94.90	121224.0
95.90	7776.0
97.00	175.0
103.70	643.0
104.80	231.0
105.80	544.0
106.90	184.0
110.70	117.0
111.90	143.0
112.90	143.0
114.70	190.0
115.80	502.0
116.90	976.0
117.80	587.0
118.90	995.0
127.80	420.0
128.80	189.0
129.80	452.0
130.60	206.0
134.90	292.0
136.90	229.0
140.80	1473.0
141.90	132.0
142.80	1676.0
144.90	427.0
145.60	195.0
147.80	339.0
149.80	133.0
154.70	154.0
155.10	143.0
155.80	167.0
156.90	190.0
158.80	119.0
170.80	218.0
171.90	1007.0
172.90	1194.0
173.90	94888.0
174.90	6663.0
175.90	91984.0
176.90	5242.0
177.90	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.80	918.0
36.90	4872.0
37.90	4452.0
38.90	1688.0
39.80	144.0
43.90	1367.0
44.90	1000.0
45.80	158.0
47.00	1202.0
47.70	534.0
48.90	4160.0
50.00	20296.0
50.90	6510.0
52.10	196.0
55.00	303.0
55.90	1917.0
56.90	3109.0
57.90	146.0
59.90	1056.0
60.90	5824.0
61.90	6103.0
62.90	4612.0
64.00	595.0
65.00	573.0
67.00	348.0
67.90	11508.0
69.00	13013.0
69.90	1064.0
71.90	488.0
72.90	5740.0
73.90	19928.0
74.90	59488.0
76.00	5375.0
76.90	680.0
78.00	349.0
78.80	4726.0
79.80	1230.0
80.80	4763.0
81.80	1156.0
82.80	113.0
85.60	119.0
86.00	110.0
86.90	4587.0
87.90	4167.0
88.70	156.0
90.70	368.0
91.90	3340.0
92.90	5218.0
93.90	13527.0
94.90	110912.0
96.00	6945.0
96.90	168.0
103.80	535.0
104.80	242.0
105.80	557.0
106.90	161.0
111.90	147.0
113.00	144.0
114.70	181.0
115.80	505.0
116.90	844.0
117.70	501.0
118.90	790.0
127.80	336.0
128.80	218.0
129.80	372.0
130.70	235.0
134.70	261.0
136.90	192.0
140.80	1321.0
142.00	140.0
142.80	1765.0
144.80	448.0
145.60	152.0
147.80	287.0
149.70	186.0
154.70	146.0
155.80	147.0
157.00	182.0
158.90	115.0
160.80	118.0
170.60	237.0
171.90	988.0
172.90	1188.0
173.90	89104.0
174.90	5876.0
175.90	86784.0
176.90	4986.0
177.80	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042