

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
 Data File : VU060722.D
 Acq On : 12 Sep 2024 18:24
 Operator : MD/SY
 Sample : P3918-20DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 13 05:49:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	7639	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	7351	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2291	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3765	0.303	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	60.000%		
4) 1,2-Dichloroethane-d4	5.685	65	3353	0.509	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
7) 1,2-Dichloropropane-d6	6.687	67	3048	0.667	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	134.000%		
8) Toluene-d8	7.887	98	4575	0.485	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	96.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1592	0.398	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	80.000%		
Target Compounds						
					Qvalue	
6) Trichloroethene	6.544	95	5843	1.259	ug/L	97
12) 1,2,3-Trichloropropane	10.865	75	46	0.017	ug/L #	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
Data File : VU060722.D
Acq On : 12 Sep 2024 18:24
Operator : MD/SY
Sample : P3918-20DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 13 05:49:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

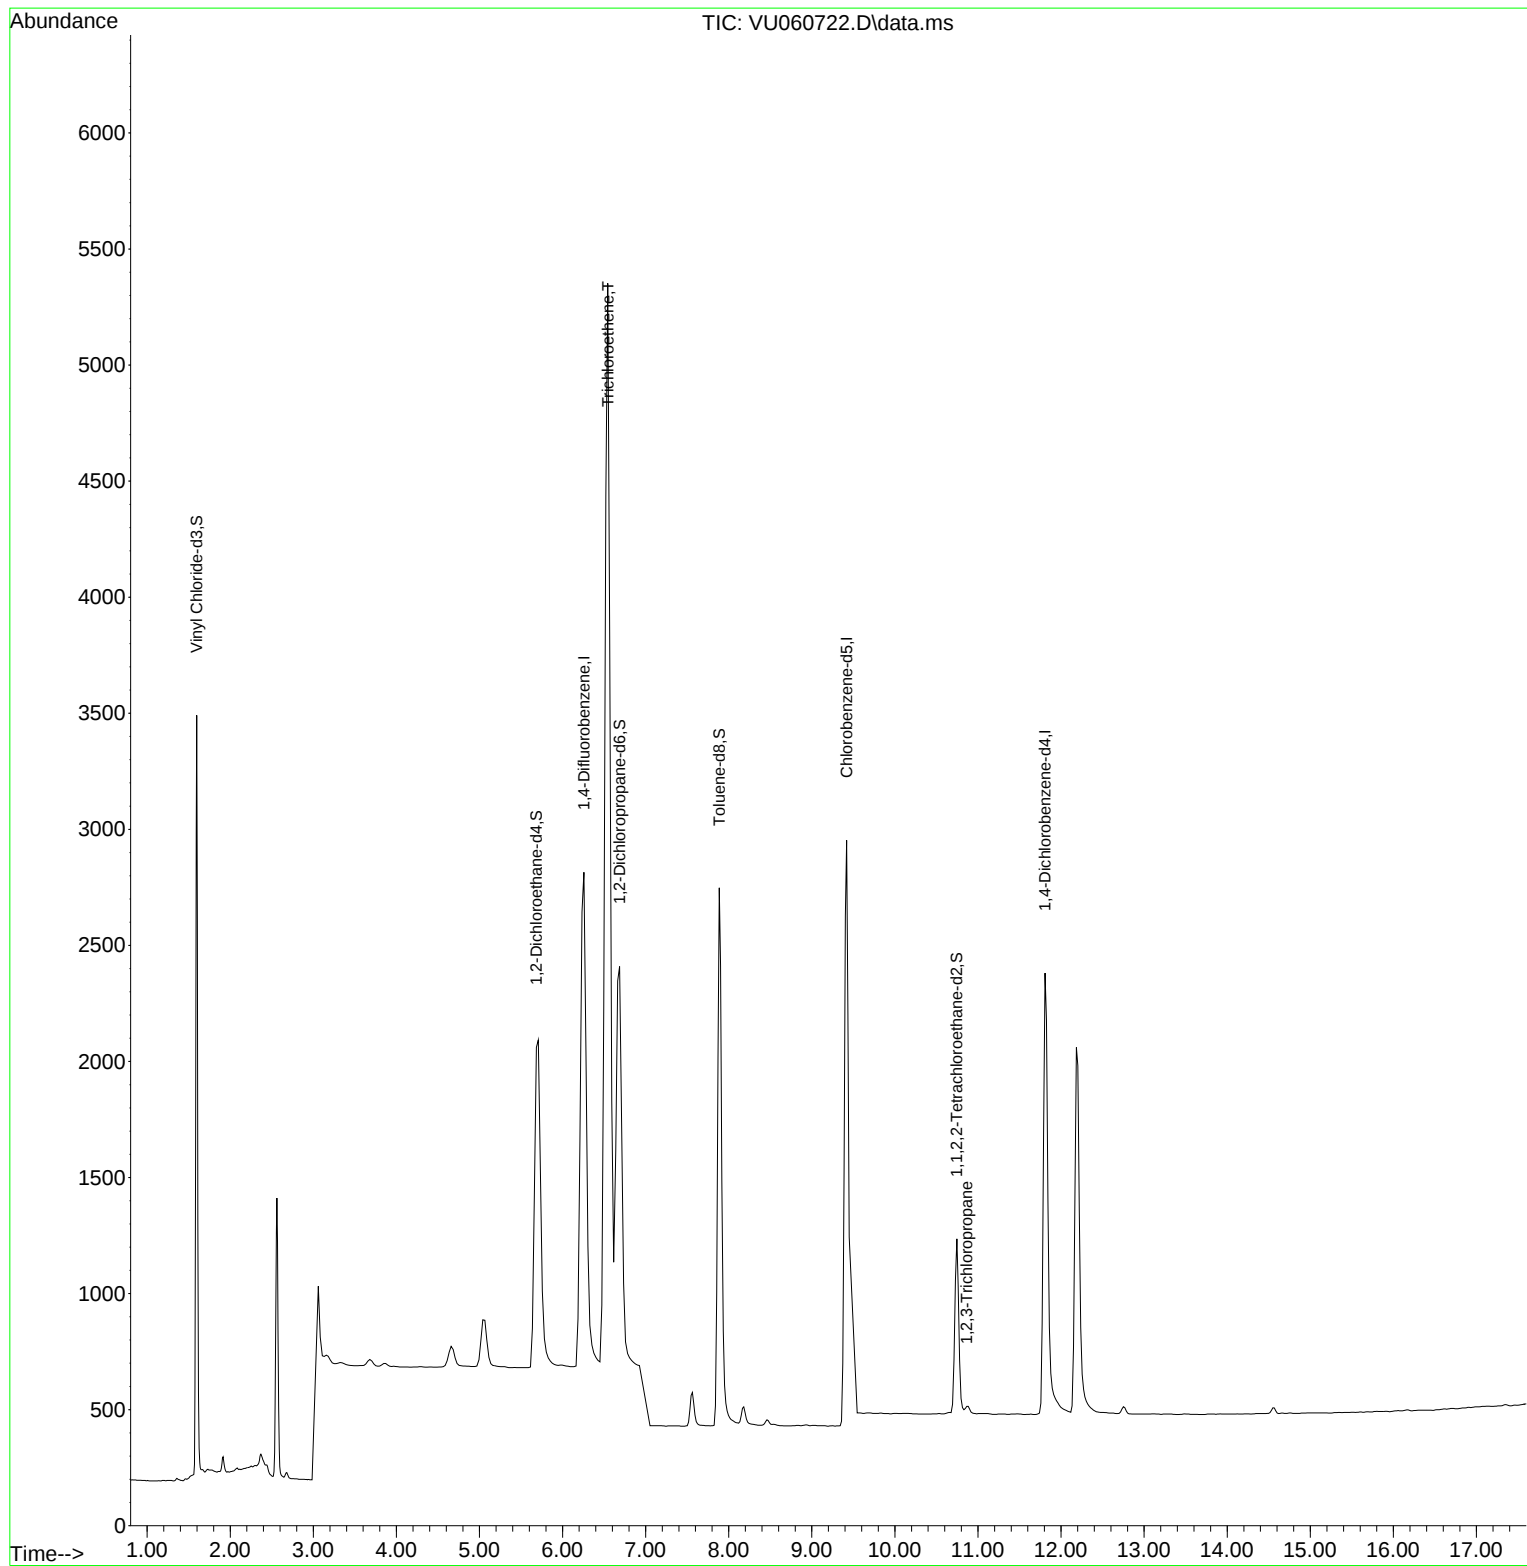

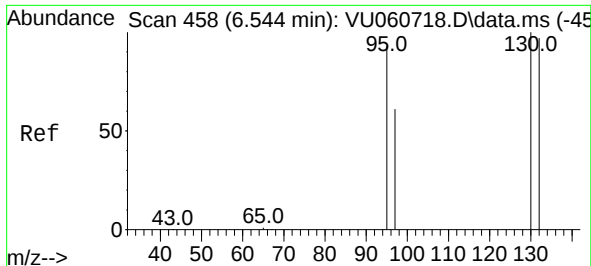



#6
 Trichloroethene
 Concen: 1.259 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. 0.000 min
 Lab File: VU060722.D
 Acq: 12 Sep 2024 18:24

Instrument :
 MSVOA_U
 ClientSampleId :

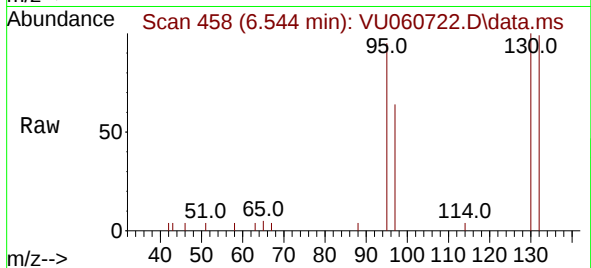


Tgt Ion: 95 Resp: 5843

Ion	Ratio	Lower	Upper
95	100		
97	67.4	48.5	90.1
132	104.2	75.5	140.1
130	105.2	76.3	141.7

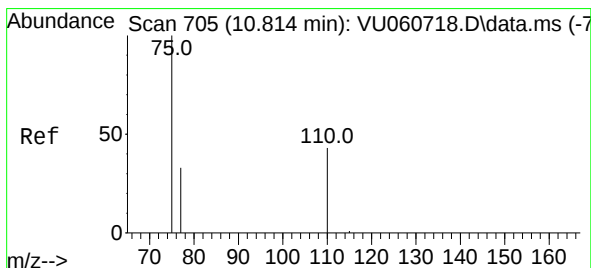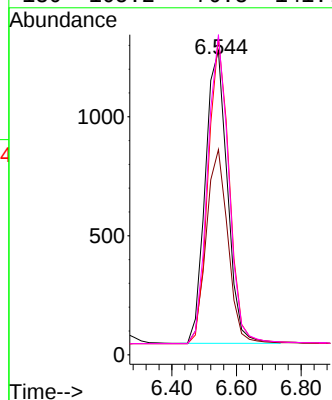

#12
 1,2,3-Trichloropropane
 Concen: 0.017 ug/L
 RT: 10.865 min Scan# 708
 Delta R.T. 0.051 min
 Lab File: VU060722.D
 Acq: 12 Sep 2024 18:24

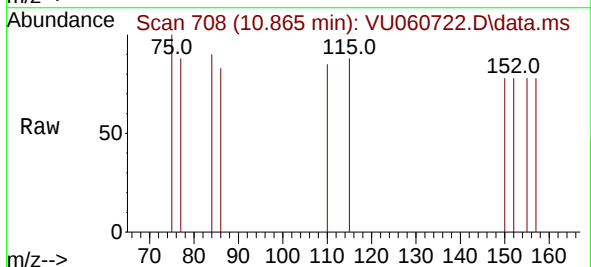

Tgt Ion: 75 Resp: 46

Ion	Ratio	Lower	Upper
75	100		
110	32.6	32.4	48.6
77	8.7	26.0	39.0

