

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
 Data File : VU060729.D
 Acq On : 12 Sep 2024 21:14
 Operator : MD/SY
 Sample : P3967-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 13 05:50:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	8478	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	12543	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	3775	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	6098	0.442	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	88.000%		
4) 1,2-Dichloroethane-d4	5.685	65	3794	0.519	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	104.000%		
7) 1,2-Dichloropropane-d6	6.687	67	3960	0.508	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	102.000%		
8) Toluene-d8	7.887	98	8566	0.532	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	106.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	3315	0.485	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	98.000%		
Target Compounds						
12) 1,2,3-Trichloropropane	10.865	75	91	0.021	ug/L	Qvalue # 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
Data File : VU060729.D
Acq On : 12 Sep 2024 21:14
Operator : MD/SY
Sample : P3967-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 13 05:50:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

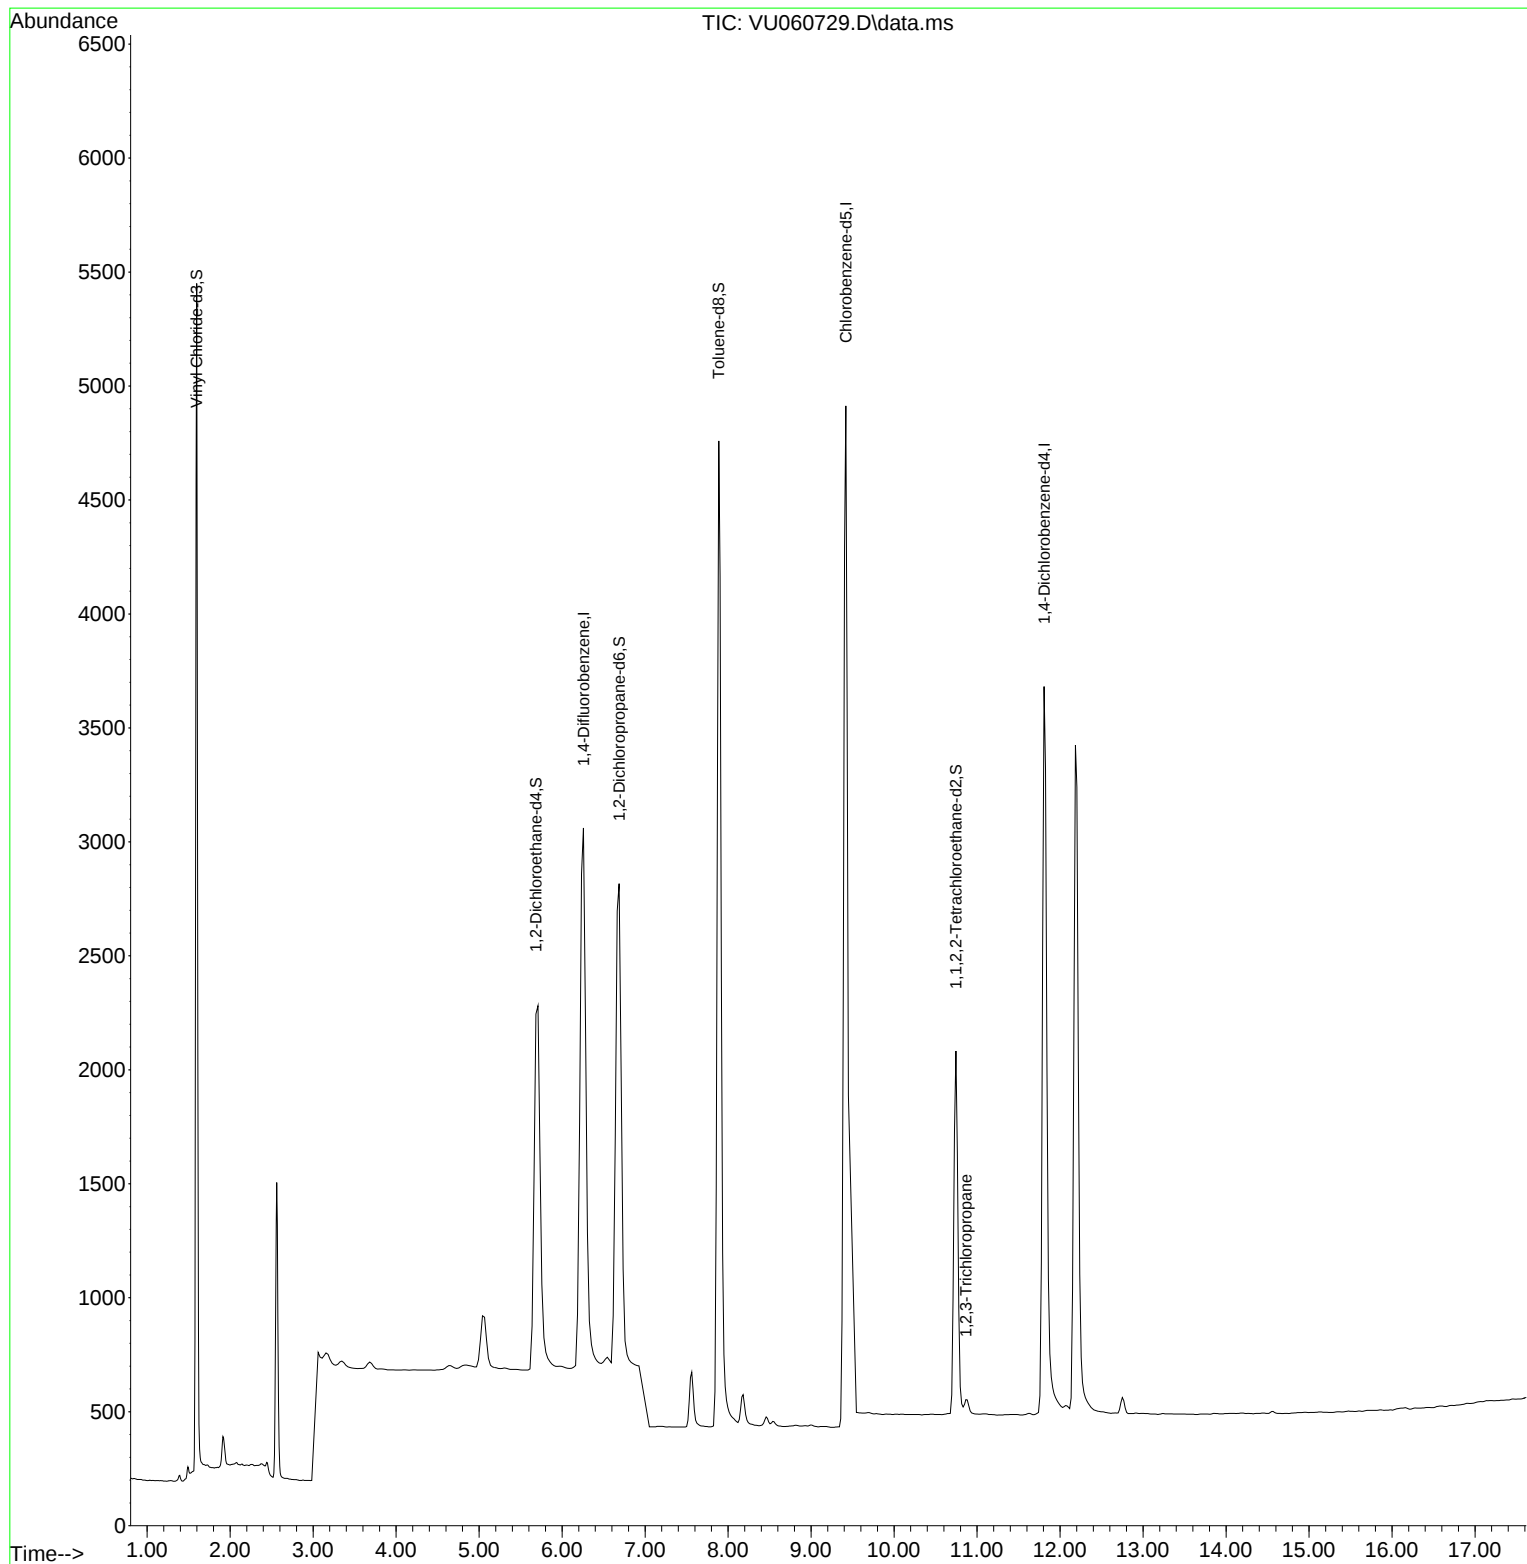

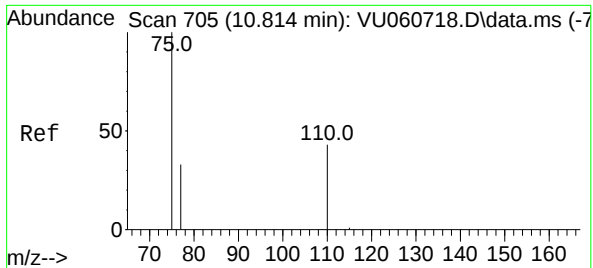

#12
 1,2,3-Trichloropropane
 Concen: 0.021 ug/L
 RT: 10.865 min Scan# 70
 Delta R.T. 0.051 min
 Lab File: VU060729.D
 Acq: 12 Sep 2024 21:14

Instrument :
 MSVOA_U
 ClientSampleId :

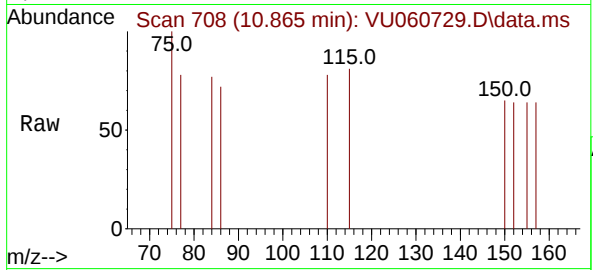

Tgt Ion: 75	Resp:	91
Ion Ratio	Lower	Upper
75	100	
110	47.3	32.4 48.6
77	5.5	26.0 39.0#

