

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
 Data File : VU060743.D
 Acq On : 13 Sep 2024 09:38
 Operator : MD/SY
 Sample : P3918-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 13 10:39:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	8167	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	11854	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	3480	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	5960	0.449	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 90.000%			
4) 1,2-Dichloroethane-d4	5.709	65	3748	0.532	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 106.000%			
7) 1,2-Dichloropropane-d6	6.687	67	4046	0.549	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 110.000%			
8) Toluene-d8	7.887	98	8943	0.587	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 118.000%			
10) 1,1,2,2-Tetrachloroeth...	10.745	84	3357	0.520	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 104.000%			
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.750	75	147	0.187	ug/L	Qvalue # 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
Data File : VU060743.D
Acq On : 13 Sep 2024 09:38
Operator : MD/SY
Sample : P3918-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 13 10:39:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

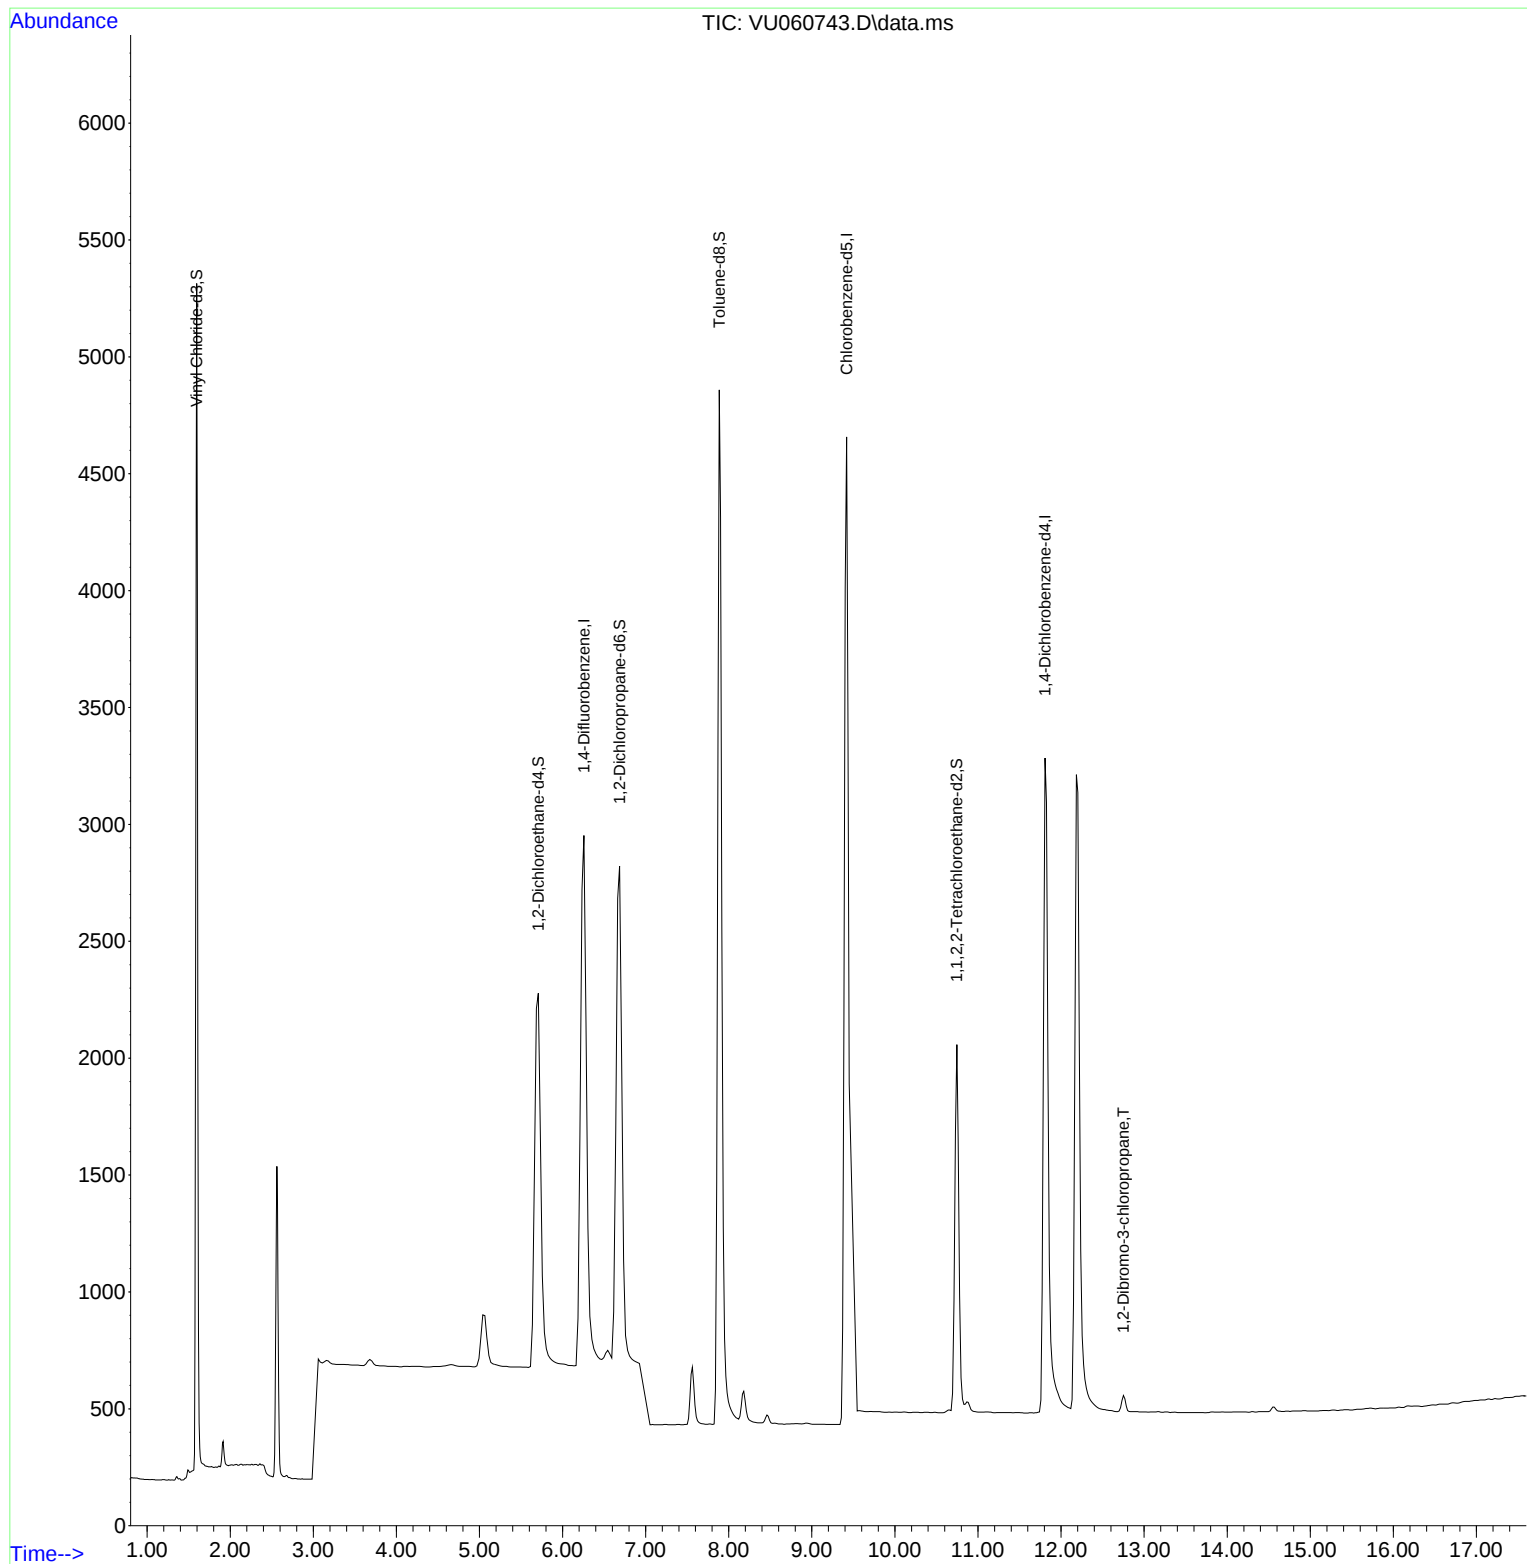

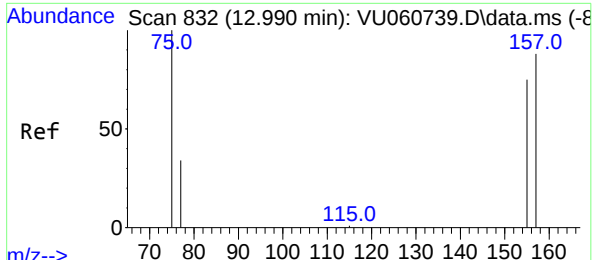

#13
1,2-Dibromo-3-chloropropane
Concen: 0.187 ug/L
RT: 12.750 min Scan# 81
Delta R.T. -0.240 min
Lab File: VU060743.D
Acq: 13 Sep 2024 09:38

Instrument :
MSVOA_U
ClientSampleId :

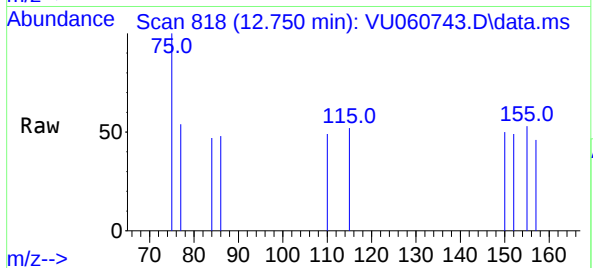

Tgt Ion: 75 Resp: 147
Ion Ratio Lower Upper
75 100
157 45.5 74.3 111.5#
155 53.5 66.2 99.2#

