

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
 Data File : VU060721.D
 Acq On : 12 Sep 2024 18:00
 Operator : MD/SY
 Sample : P3918-14DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN9DL

Quant Time: Sep 13 05:49:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	6767	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	7610	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2389	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	4810	0.437	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	88.000%		
4) 1,2-Dichloroethane-d4	5.685	65	2981	0.511	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
7) 1,2-Dichloropropane-d6	6.687	67	2835	0.599	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	120.000%		
8) Toluene-d8	7.888	98	4788	0.490	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	98.000%		
10) 1,1,2,2-Tetrachloroeth...	10.746	84	1704	0.411	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	82.000%		
Target Compounds						
6) Trichloroethene	6.544	95	4898	1.019	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
Data File : VU060721.D
Acq On : 12 Sep 2024 18:00
Operator : MD/SY
Sample : P3918-14DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN9DL


Quant Time: Sep 13 05:49:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

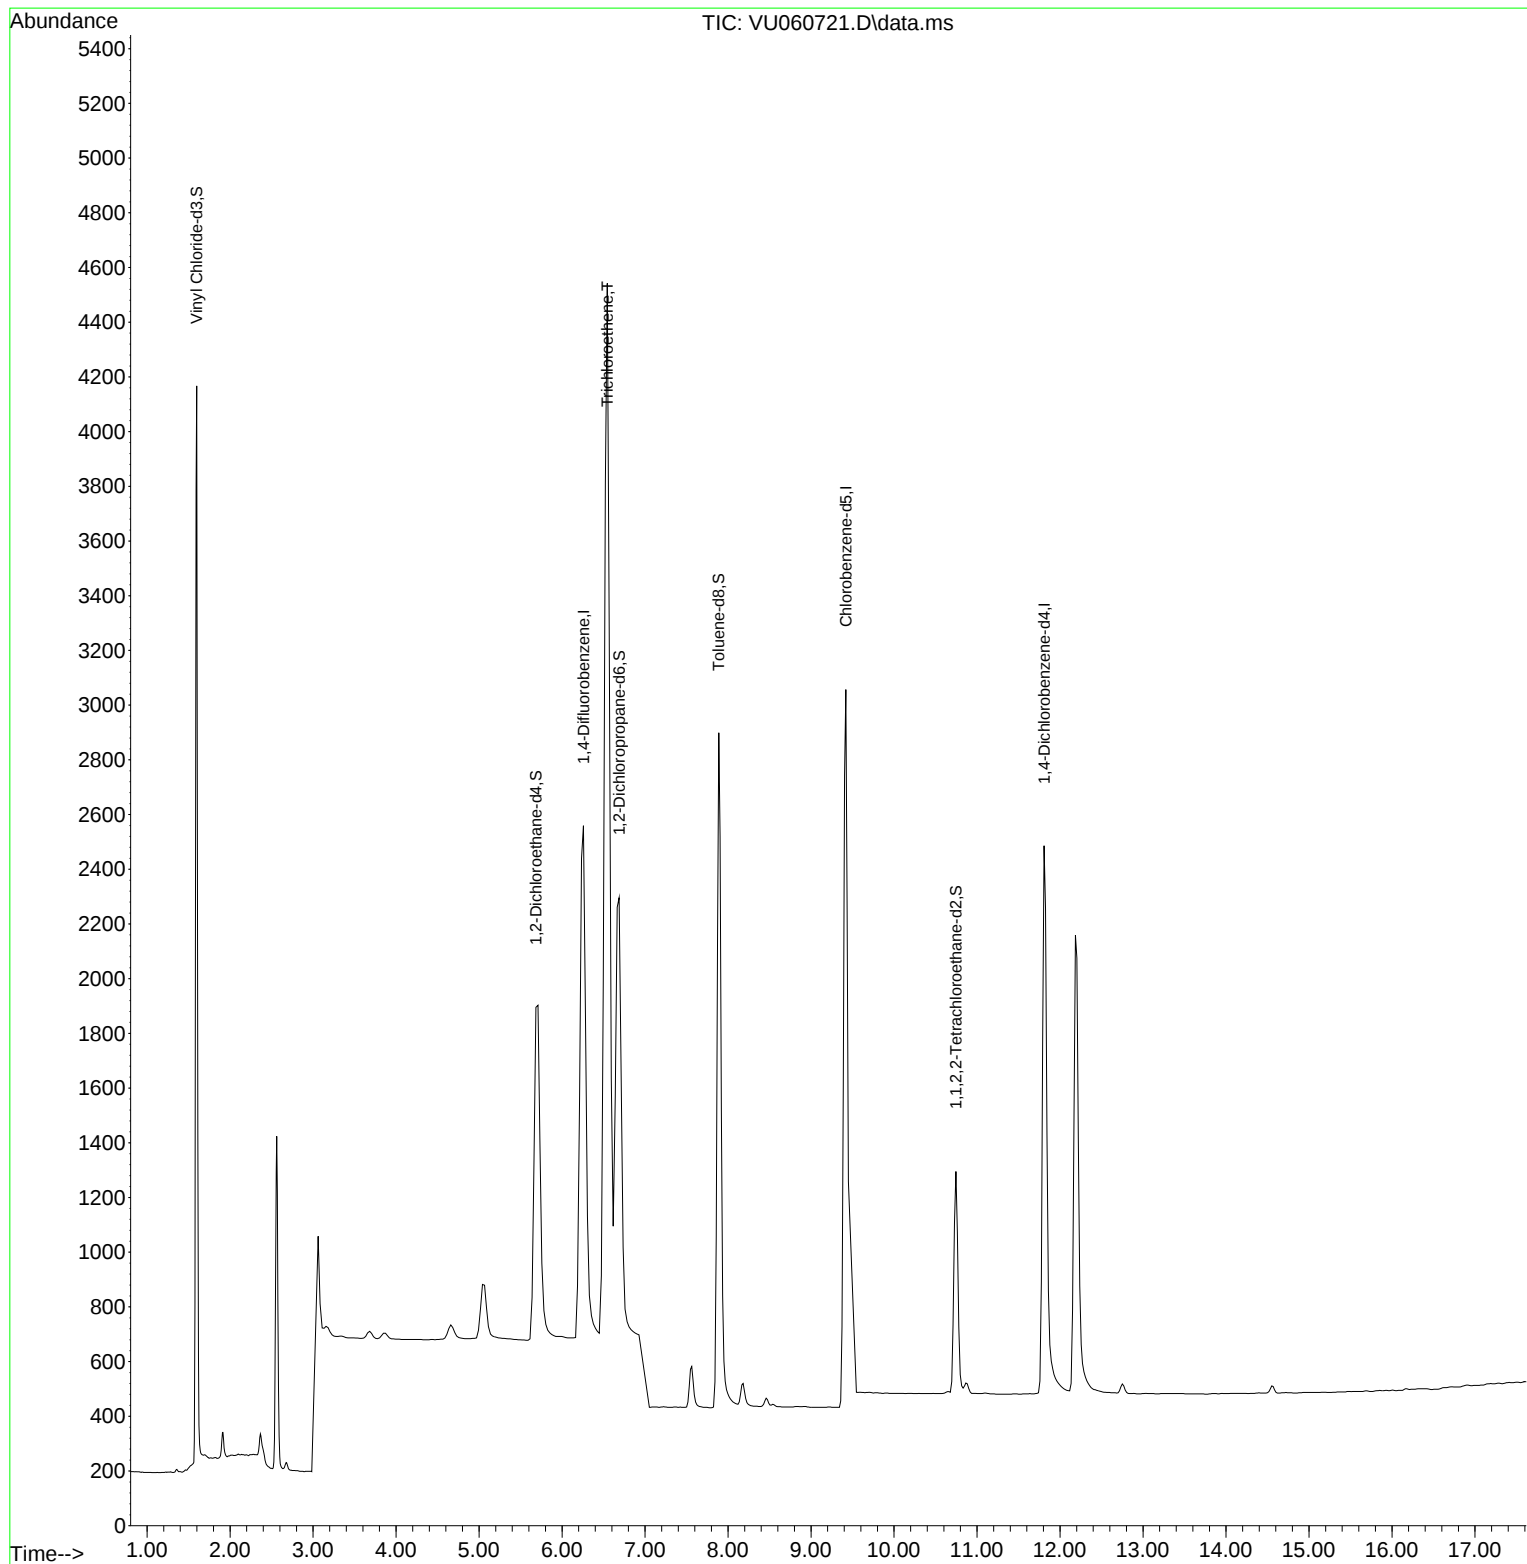

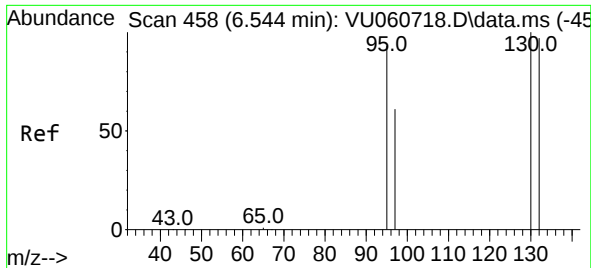

#6
 Trichloroethene
 Concen: 1.019 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. 0.000 min
 Lab File: VU060721.D
 Acq: 12 Sep 2024 18:00

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN9DL

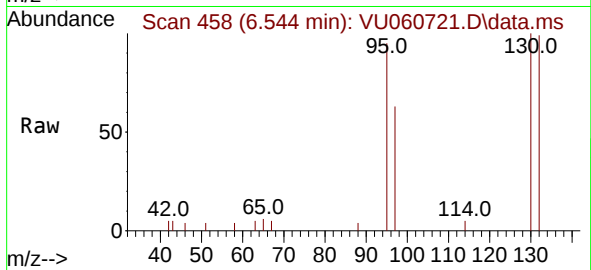

Tgt Ion: 95	Resp: 4898
Ion Ratio	Lower Upper
95 100	
97 66.4	48.5 90.1
132 103.6	75.5 140.1
130 105.0	76.3 141.7

