

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
 Data File : VU060723.D
 Acq On : 12 Sep 2024 18:48
 Operator : MD/SY
 Sample : P3918-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP6

Quant Time: Sep 13 05:49:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	5085	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	7641	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	3084	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	4418	0.534	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 106.000%			
4) 1,2-Dichloroethane-d4	5.709	65	2117	0.483	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 96.000%			
7) 1,2-Dichloropropane-d6	6.687	67	1854	0.390	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 78.000%			
8) Toluene-d8	7.887	98	4526	0.461	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 92.000%			
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1550	0.373	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 74.000%			
Target Compounds					Qvalue	
6) Trichloroethene	6.544	95	153	0.032	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
Data File : VU060723.D
Acq On : 12 Sep 2024 18:48
Operator : MD/SY
Sample : P3918-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP6


Quant Time: Sep 13 05:49:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

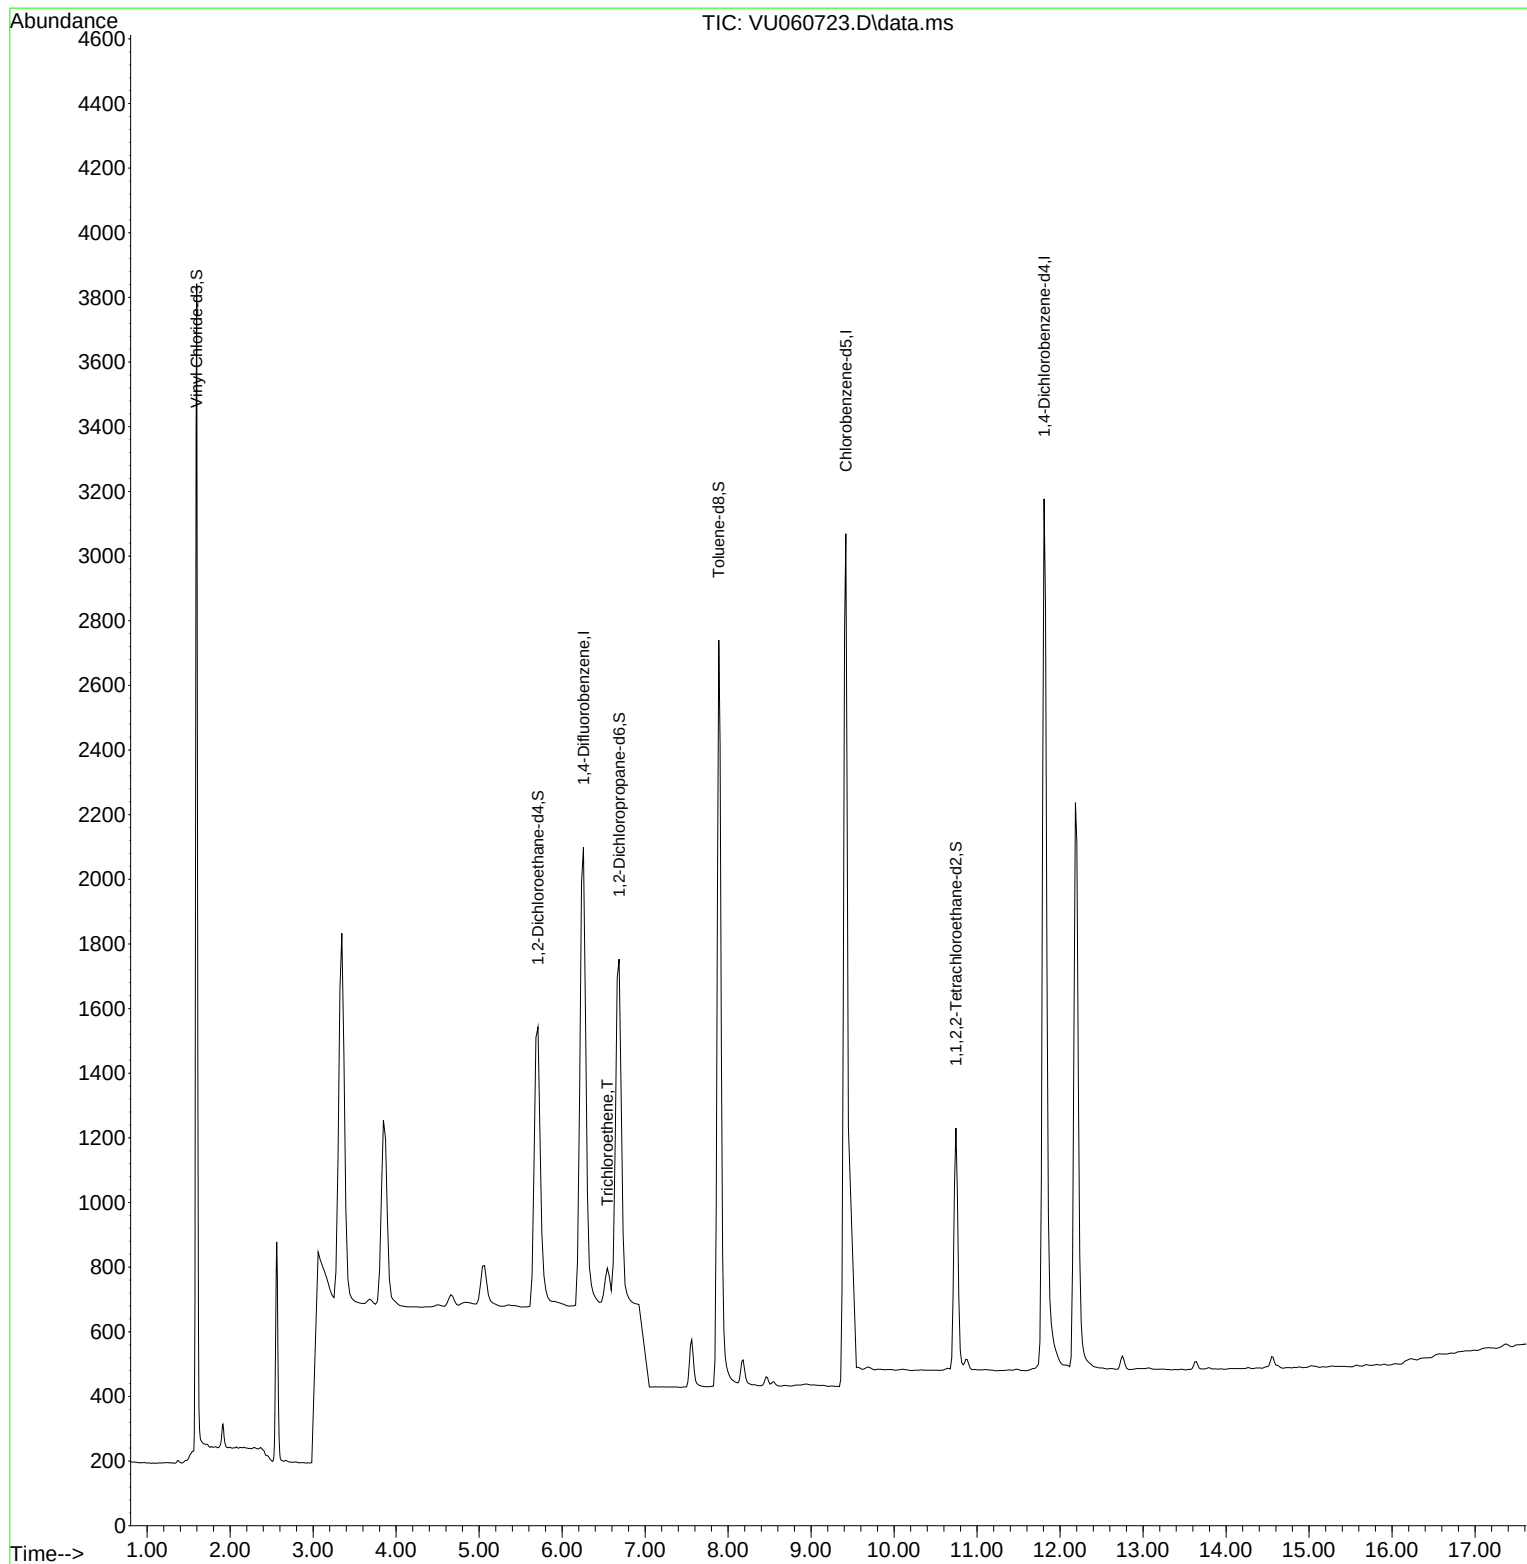

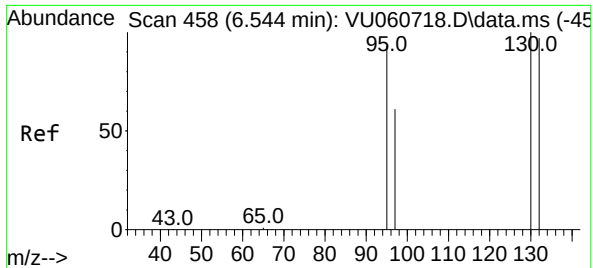

#6
 Trichloroethene
 Concen: 0.032 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. -0.000 min
 Lab File: VU060723.D
 Acq: 12 Sep 2024 18:48

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP6

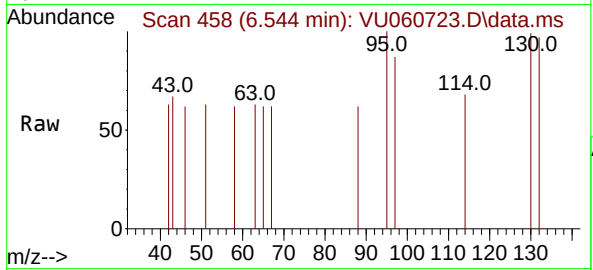

Tgt Ion: 95	Resp:	153	
Ion	Ratio	Lower	Upper
95	100		
97	87.2	48.5	90.1
132	97.4	75.5	140.1
130	98.7	76.3	141.7

