

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
 Data File : VU060724.D
 Acq On : 12 Sep 2024 19:13
 Operator : MD/SY
 Sample : P3918-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP7

Quant Time: Sep 13 05:49:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	9046	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	12807	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	3951	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	6455	0.439	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	88.000%		
4) 1,2-Dichloroethane-d4	5.685	65	4090	0.525	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	104.000%		
7) 1,2-Dichloropropane-d6	6.687	67	4289	0.539	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	108.000%		
8) Toluene-d8	7.888	98	9378	0.570	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	114.000%		
10) 1,1,2,2-Tetrachloroeth...	10.746	84	3610	0.518	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	104.000%		
Target Compounds						
6) Trichloroethene	6.544	95	226	0.028	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
Data File : VU060724.D
Acq On : 12 Sep 2024 19:13
Operator : MD/SY
Sample : P3918-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP7


Quant Time: Sep 13 05:49:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

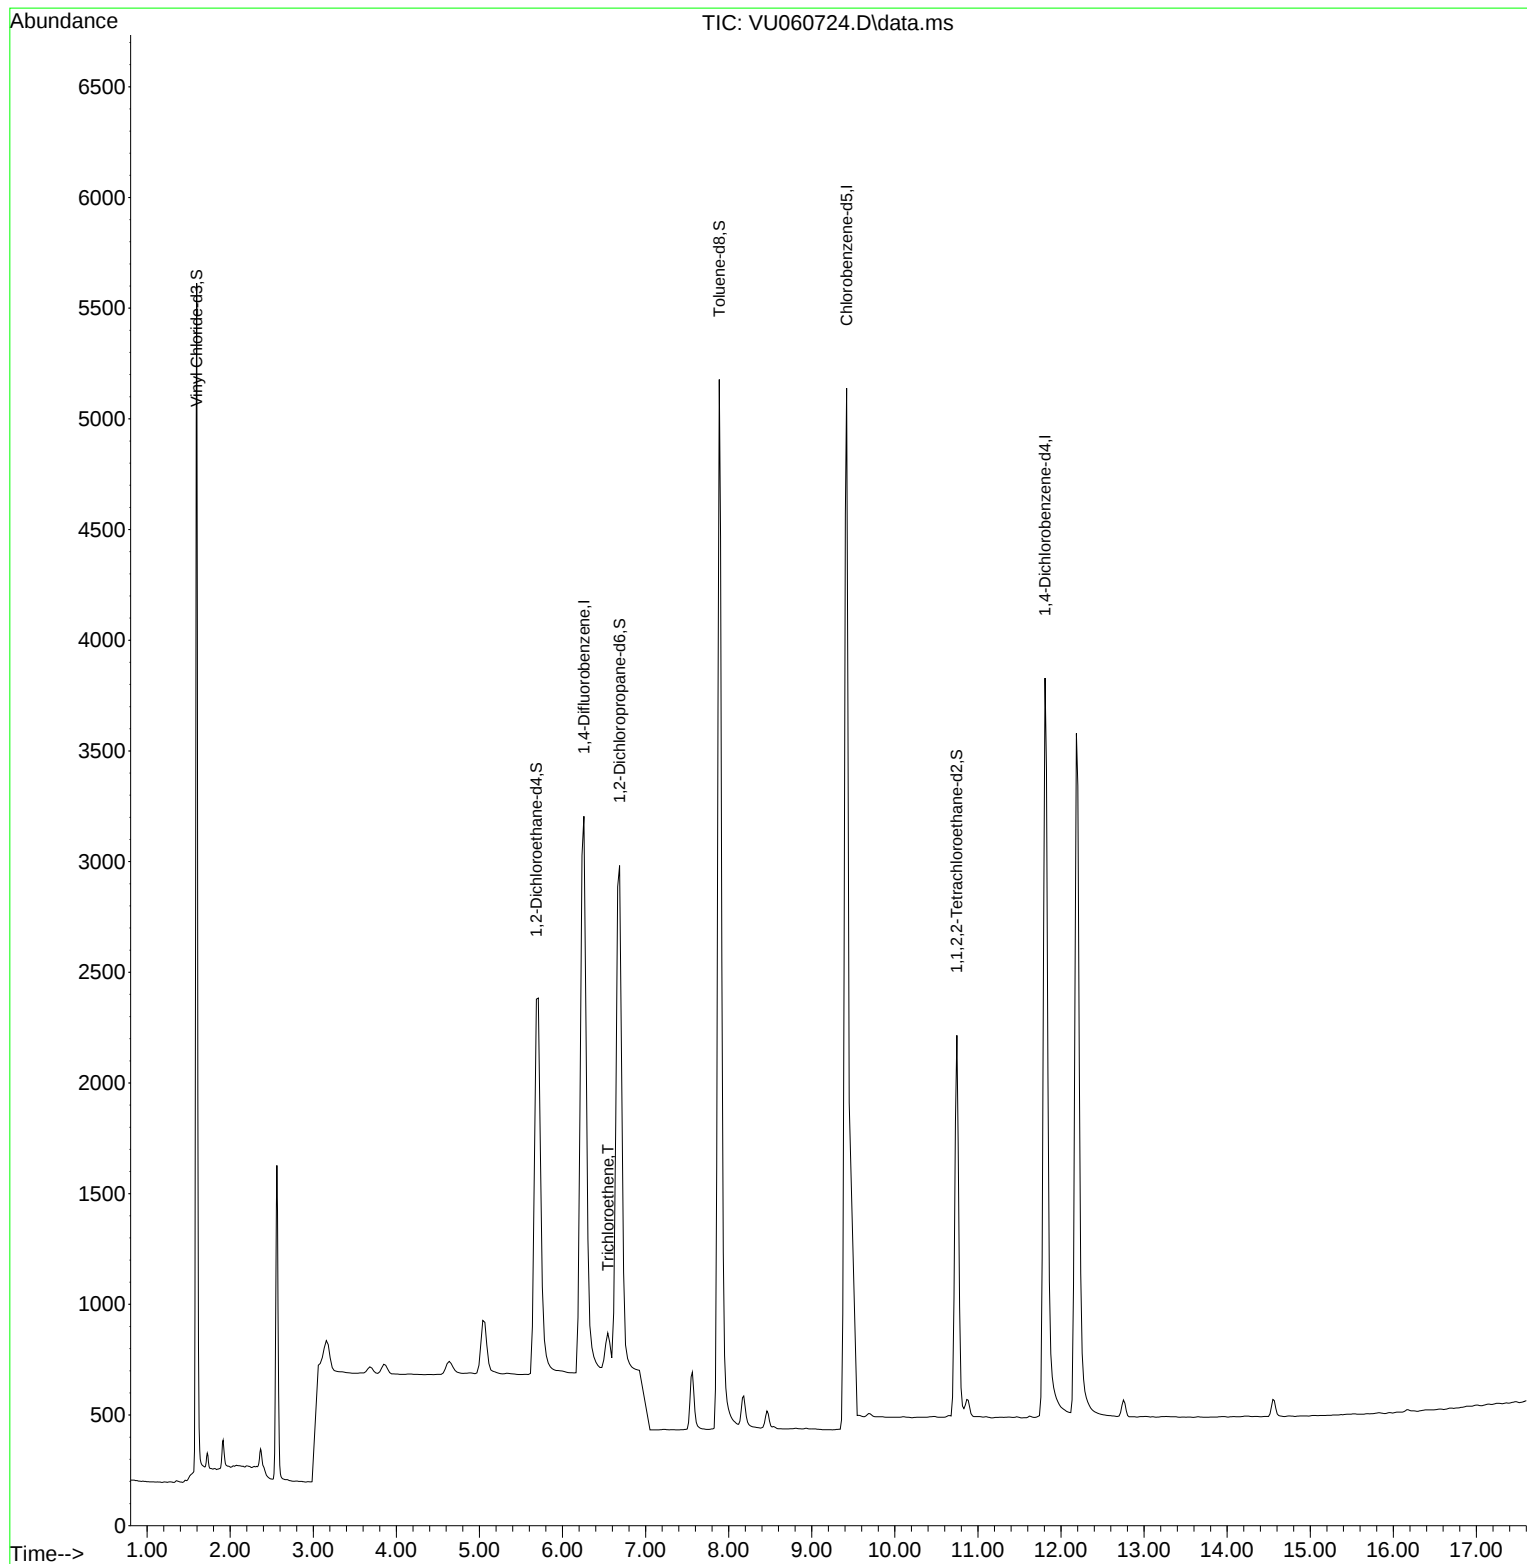

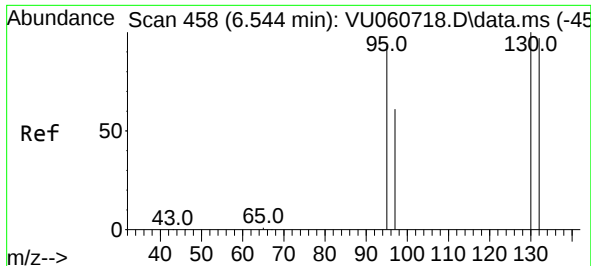

#6
Trichloroethene
Concen: 0.028 ug/L
RT: 6.544 min Scan# 41
Delta R.T. 0.000 min
Lab File: VU060724.D
Acq: 12 Sep 2024 19:13

Instrument :
MSVOA_U
ClientSampleId :
C0AP7

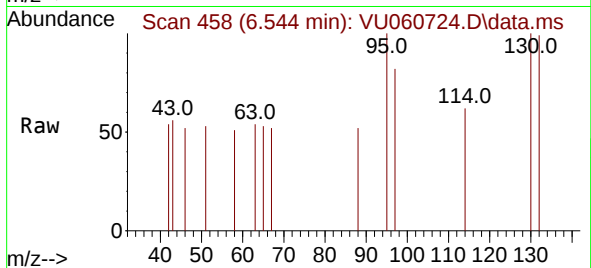

Tgt Ion: 95	Resp: 226
Ion Ratio	Lower Upper
95 100	
97 81.9	48.5 90.1
132 98.9	75.5 140.1
130 100.0	76.3 141.7

