

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
 Data File : VU060730.D
 Acq On : 12 Sep 2024 21:38
 Operator : MD/SY
 Sample : P3967-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AQ0

Quant Time: Sep 13 05:50:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	8521	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	12593	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	3712	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	5801	0.418	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	84.000%		
4) 1,2-Dichloroethane-d4	5.685	65	3608	0.491	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	98.000%		
7) 1,2-Dichloropropane-d6	6.687	67	3727	0.476	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	96.000%		
8) Toluene-d8	7.887	98	8154	0.504	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	100.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	3188	0.465	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	92.000%		
Target Compounds						
6) Trichloroethene	6.544	95	8826	1.110	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
Data File : VU060730.D
Acq On : 12 Sep 2024 21:38
Operator : MD/SY
Sample : P3967-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AQ0


Quant Time: Sep 13 05:50:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

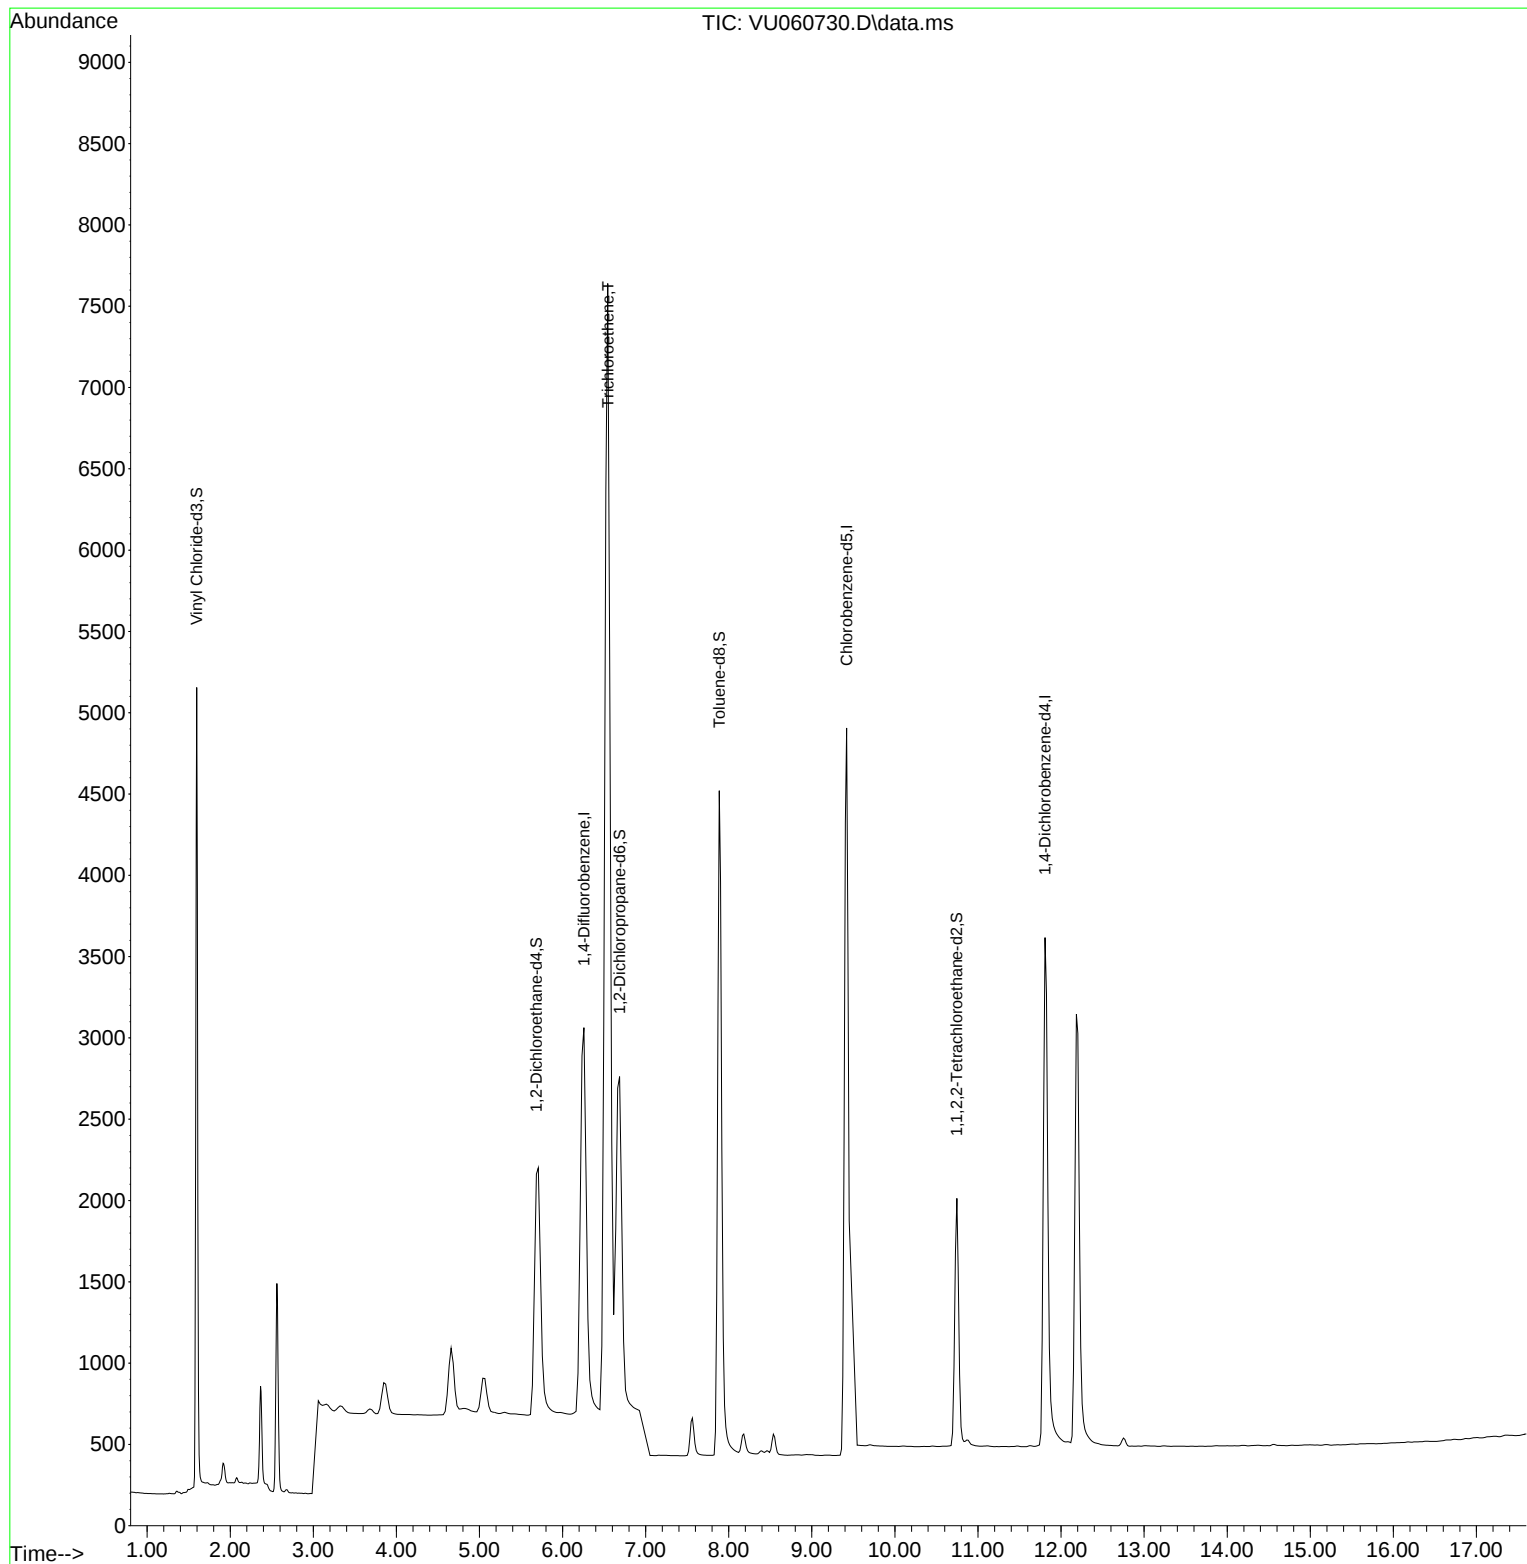

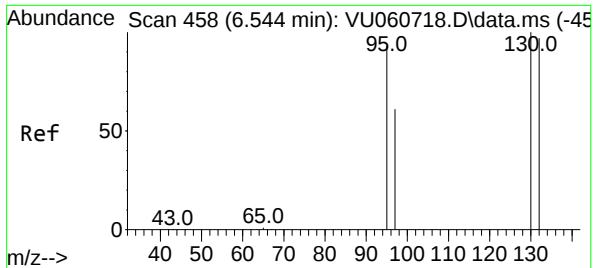

#6
 Trichloroethene
 Concen: 1.110 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. 0.000 min
 Lab File: VU060730.D
 Acq: 12 Sep 2024 21:38

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AQ0

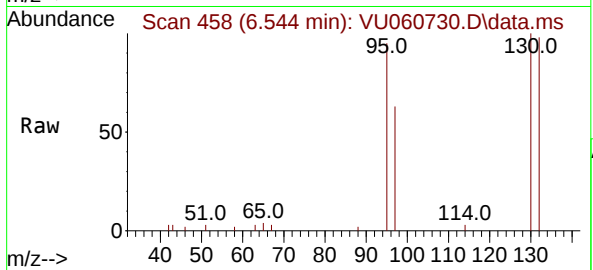

Tgt Ion: 95	Resp: 8826
Ion Ratio	Lower Upper
95 100	
97 66.3	48.5 90.1
132 103.3	75.5 140.1
130 104.9	76.3 141.7

