

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
 Data File : VU060741.D
 Acq On : 13 Sep 2024 08:50
 Operator : MD/SY
 Sample : P3967-09DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AR5DL

Quant Time: Sep 13 10:39:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	8326	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	12117	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.825	152	3539	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	5834	0.431	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	86.000%		
4) 1,2-Dichloroethane-d4	5.709	65	3626	0.505	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
7) 1,2-Dichloropropane-d6	6.687	67	3825	0.508	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	102.000%		
8) Toluene-d8	7.887	98	8792	0.565	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	112.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	3234	0.490	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	98.000%		
Target Compounds					Qvalue	
6) Trichloroethene	6.544	95	6166	0.806	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091224\
Data File : VU060741.D
Acq On : 13 Sep 2024 08:50
Operator : MD/SY
Sample : P3967-09DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AR5DL


Quant Time: Sep 13 10:39:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

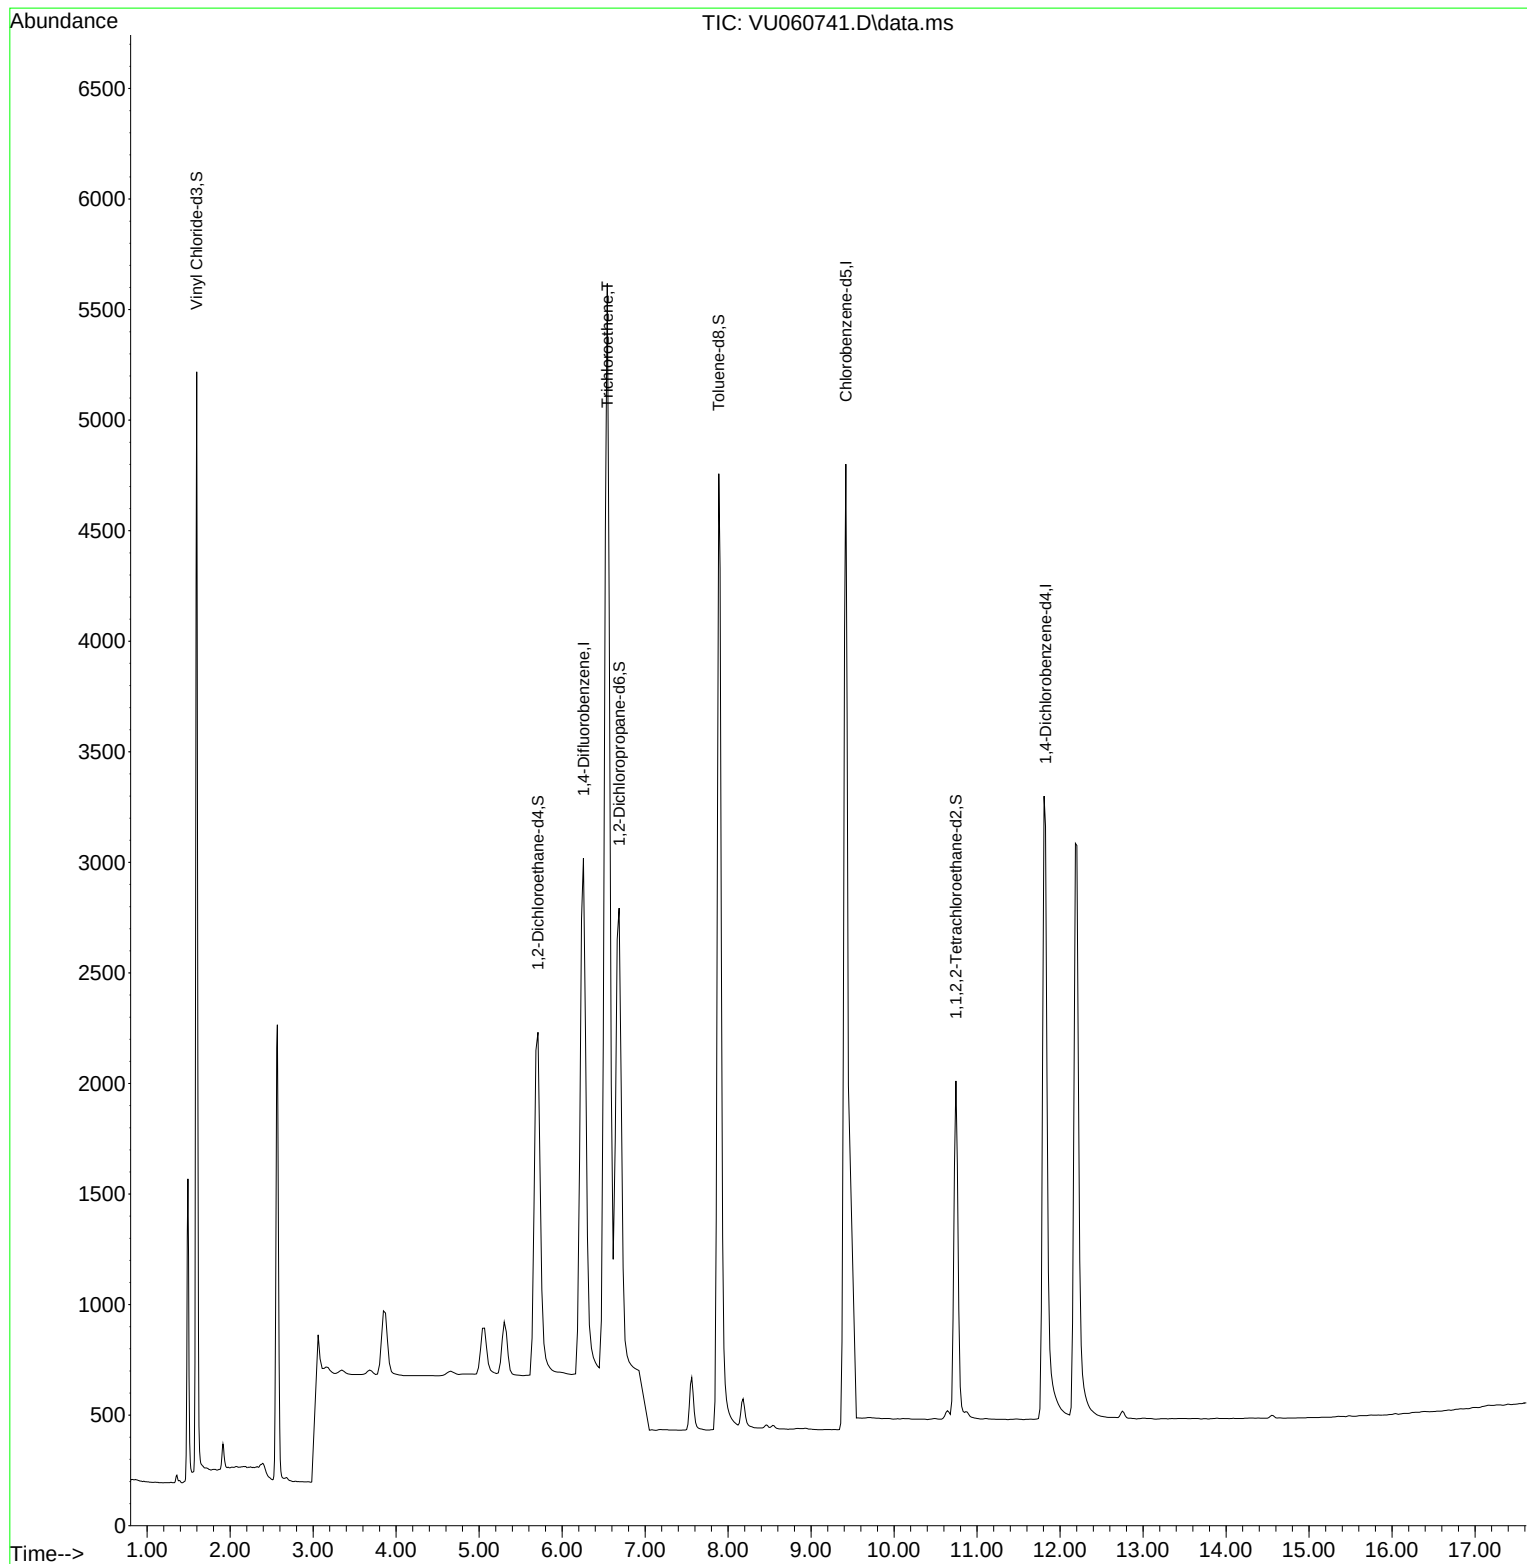

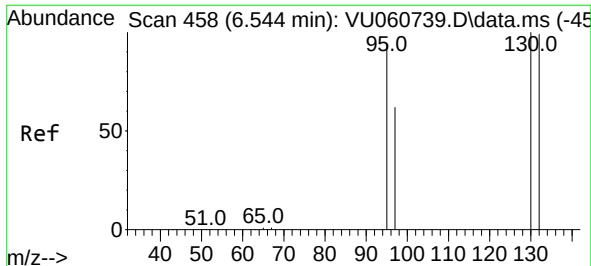

#6
 Trichloroethene
 Concen: 0.806 ug/L
 RT: 6.544 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VU060741.D
 Acq: 13 Sep 2024 08:50

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AR5DL

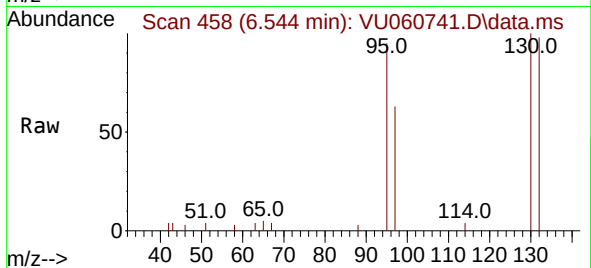

Tgt Ion: 95	Resp: 6166
Ion Ratio	Lower Upper
95 100	
97 66.6	48.5 90.1
132 103.0	75.5 140.1
130 105.2	76.3 141.7

