

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091225\
 Data File : VU063568.D
 Acq On : 12 Sep 2025 13:07
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Sep 13 03:02:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Sat Sep 13 03:01:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.100	96	34632	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	11468	0.889	ug/l	0.00
Spiked Amount 1.000			Recovery	=	89.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	11461	0.871	ug/l	0.00
Spiked Amount 1.000			Recovery	=	87.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091225\
Data File : VU063568.D
Acq On : 12 Sep 2025 13:07
Operator : MD/SY
Sample : VIBLK
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Sep 13 03:02:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Sat Sep 13 03:01:11 2025
Response via : Initial Calibration




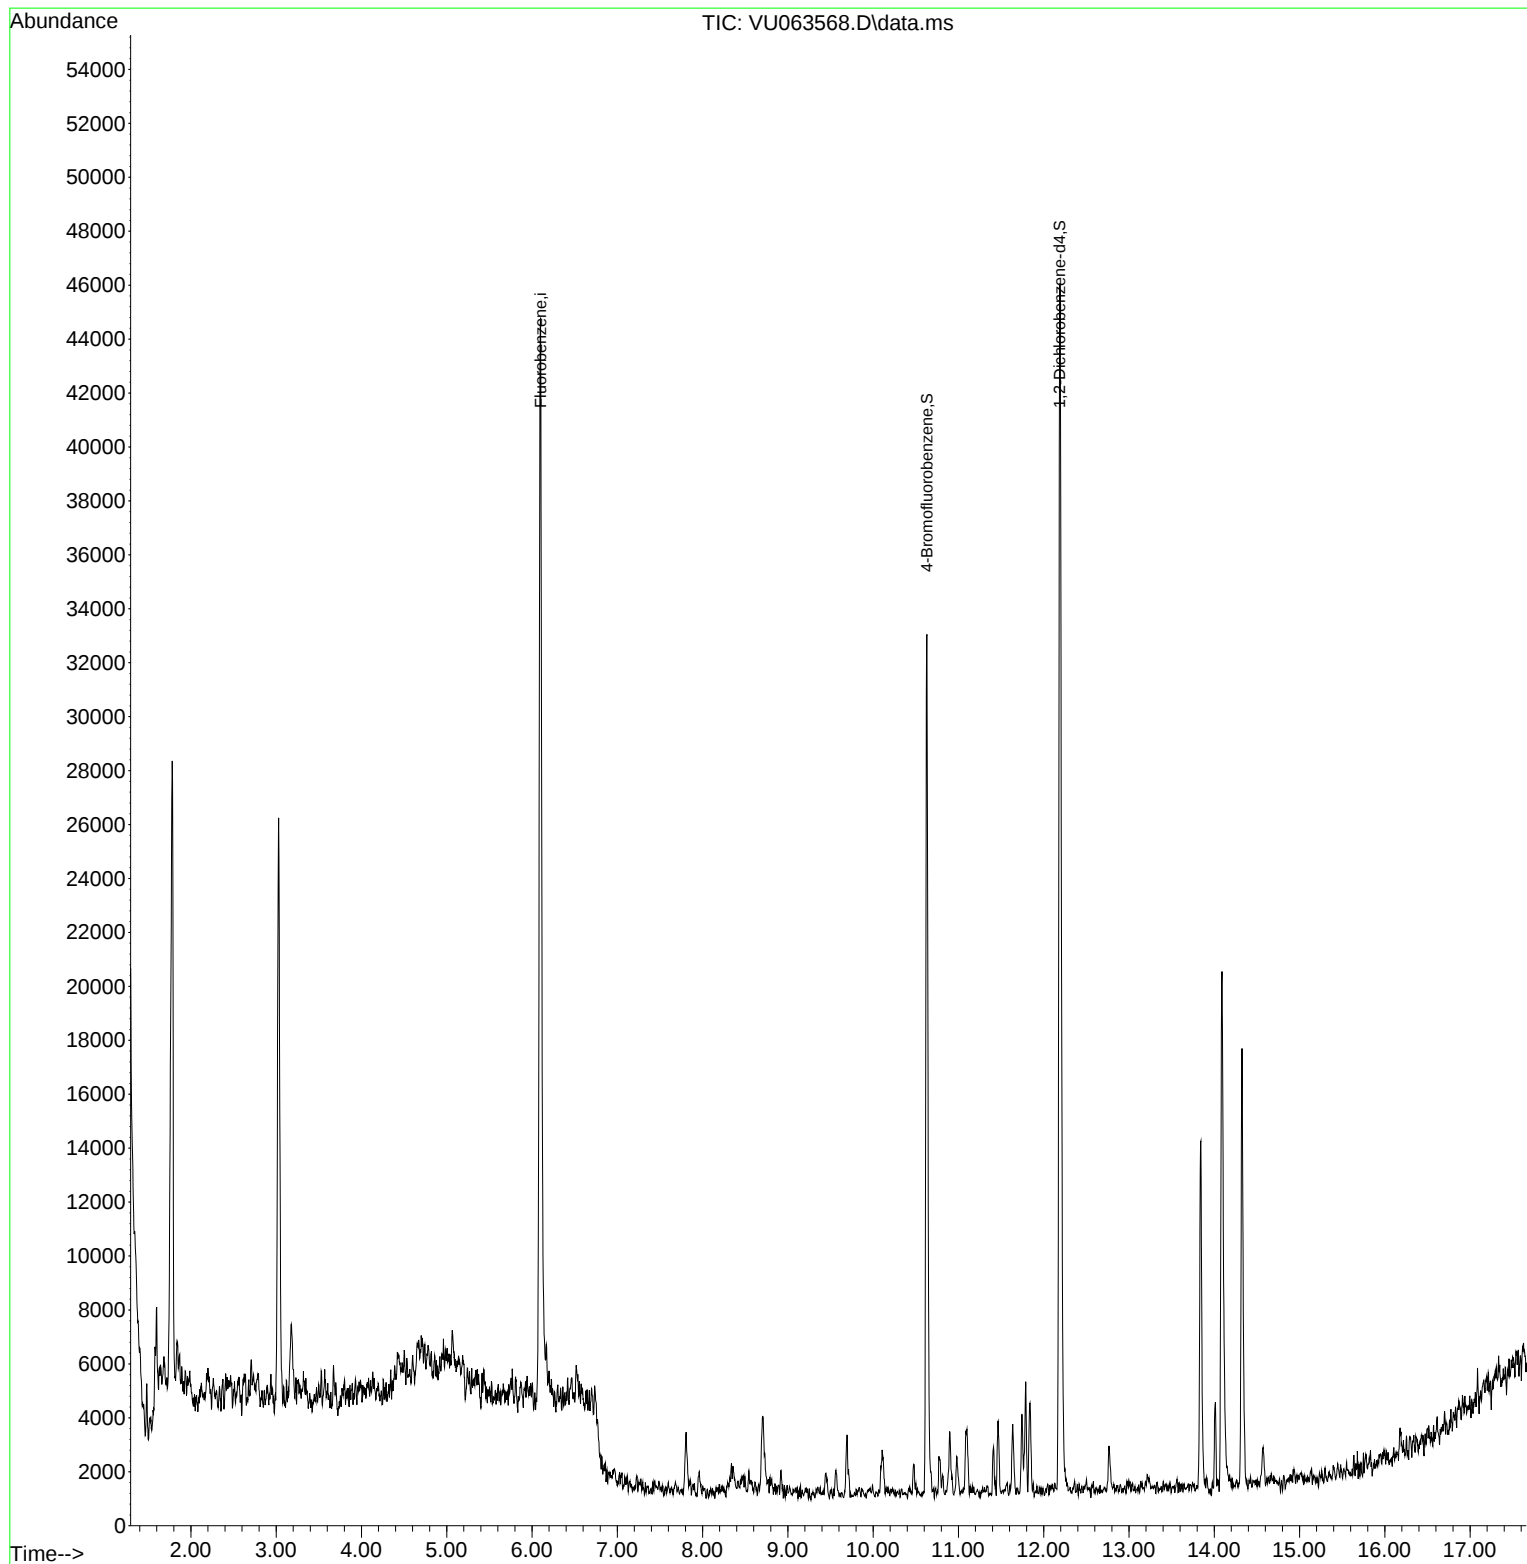


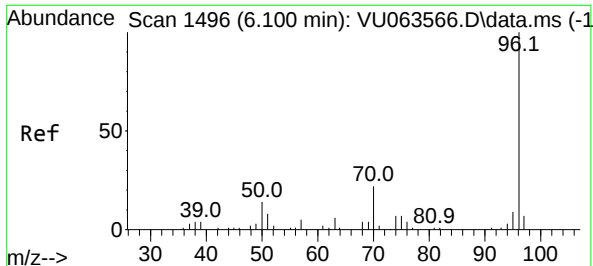

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1496
Delta R.T. 0.000 min
Lab File: VU063568.D
Acq: 12 Sep 2025 13:07




Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Tgt Ion: 96	Resp: 34632
Ion Ratio	Lower Upper
96 100	
70 21.4	15.5 23.3
95 8.3	7.7 11.5
97 6.4	0.0 0.0#

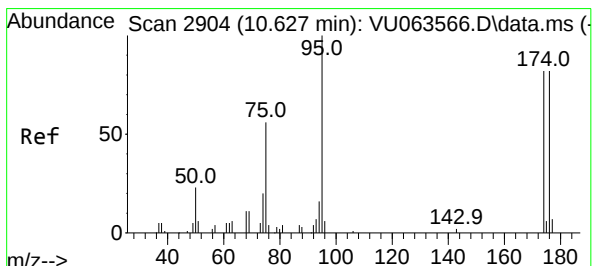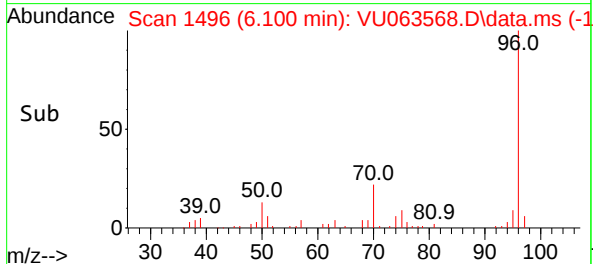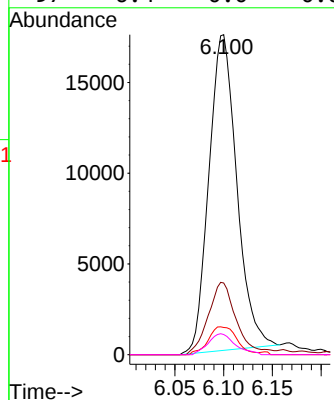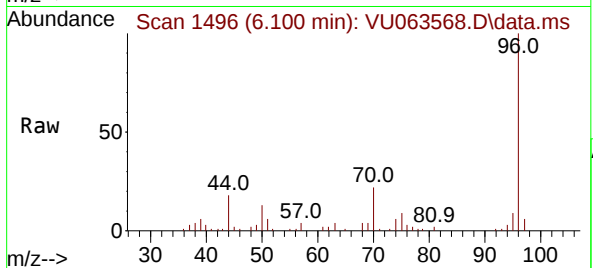

#57
4-Bromofluorobenzene
Concen: 0.889 ug/l
RT: 10.630 min Scan# 2905
Delta R.T. 0.003 min
Lab File: VU063568.D
Acq: 12 Sep 2025 13:07

Tgt Ion: 95	Resp: 11468
Ion Ratio	Lower Upper
95 100	
174 82.1	64.7 97.1
176 73.2	66.2 99.4

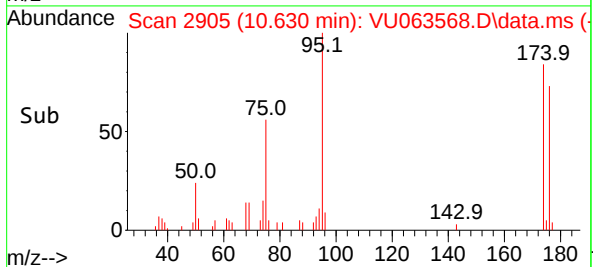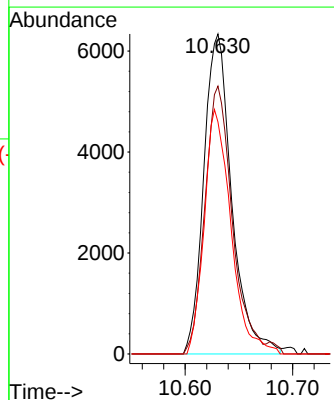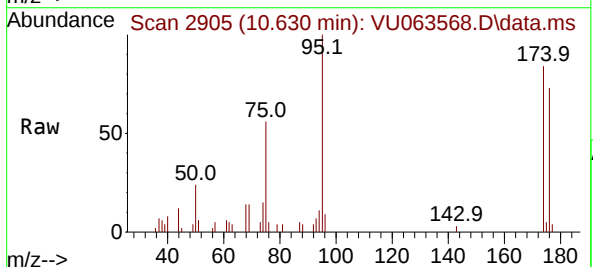

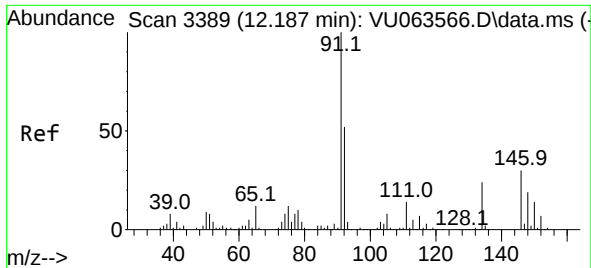

#68

1,2-Dichlorobenzene-d4

Concen: 0.871 ug/l

RT: 12.187 min Scan# 31

Delta R.T. -0.000 min

Lab File: VU063568.D


Acq: 12 Sep 2025 13:07

Instrument :

MSVOA_U

ClientSampleId :

VIBLK

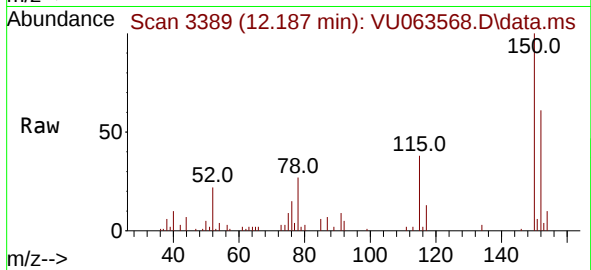

Tgt Ion:152 Resp: 11461

Ion Ratio Lower Upper

152 100

115 62.7 0.0 260.6

150 163.5 0.0 661.8

