


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091225\
Data File : VU063561.D
Acq On : 12 Sep 2025 07:52
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Sat Sep 13 03:31:19 2025

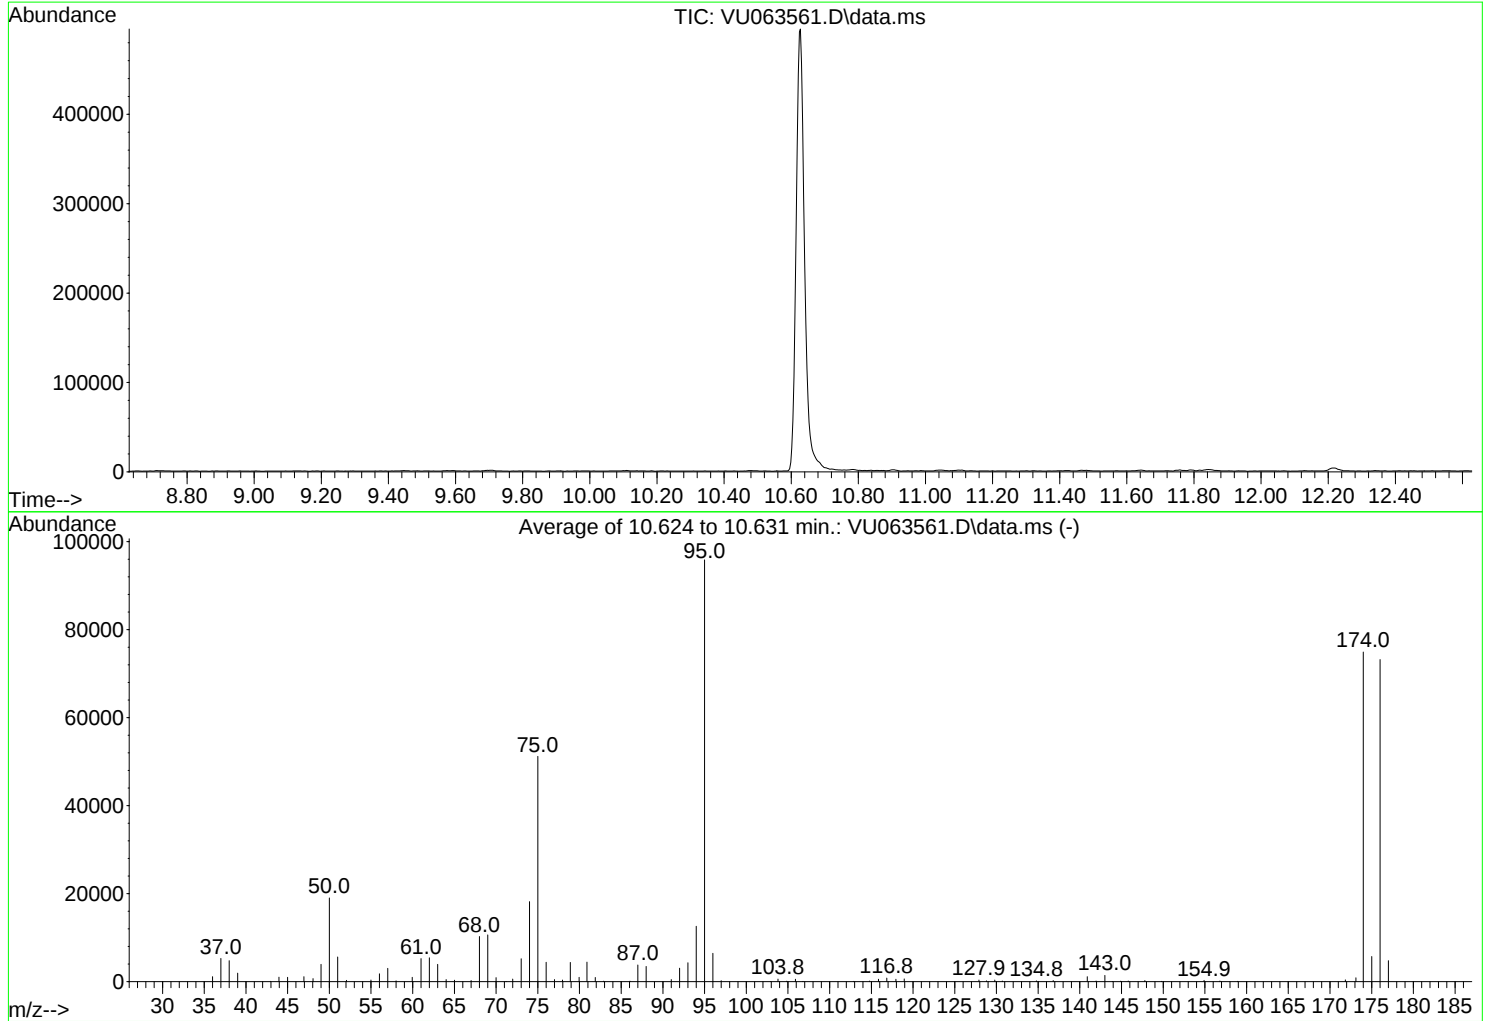

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	19008	PASS
75	95	30	60	53.4	51184	PASS
95	95	100	100	100.0	95864	PASS
96	95	5	9	6.7	6449	PASS
173	174	0.00	2	1.2	862	PASS
174	95	50	100	78.1	74915	PASS
175	174	5	9	7.7	5731	PASS
176	174	95	101	97.7	73189	PASS
177	176	5	9	6.5	4782	PASS