


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091318\
 Data File : VU026696.D
 Acq On : 12 Sep 2018 12:28
 Operator : MD/SY
 Sample : BFB40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB40

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
 Title : VOC Analysis
 Last Update : Thu Sep 13 03:38:50 2018

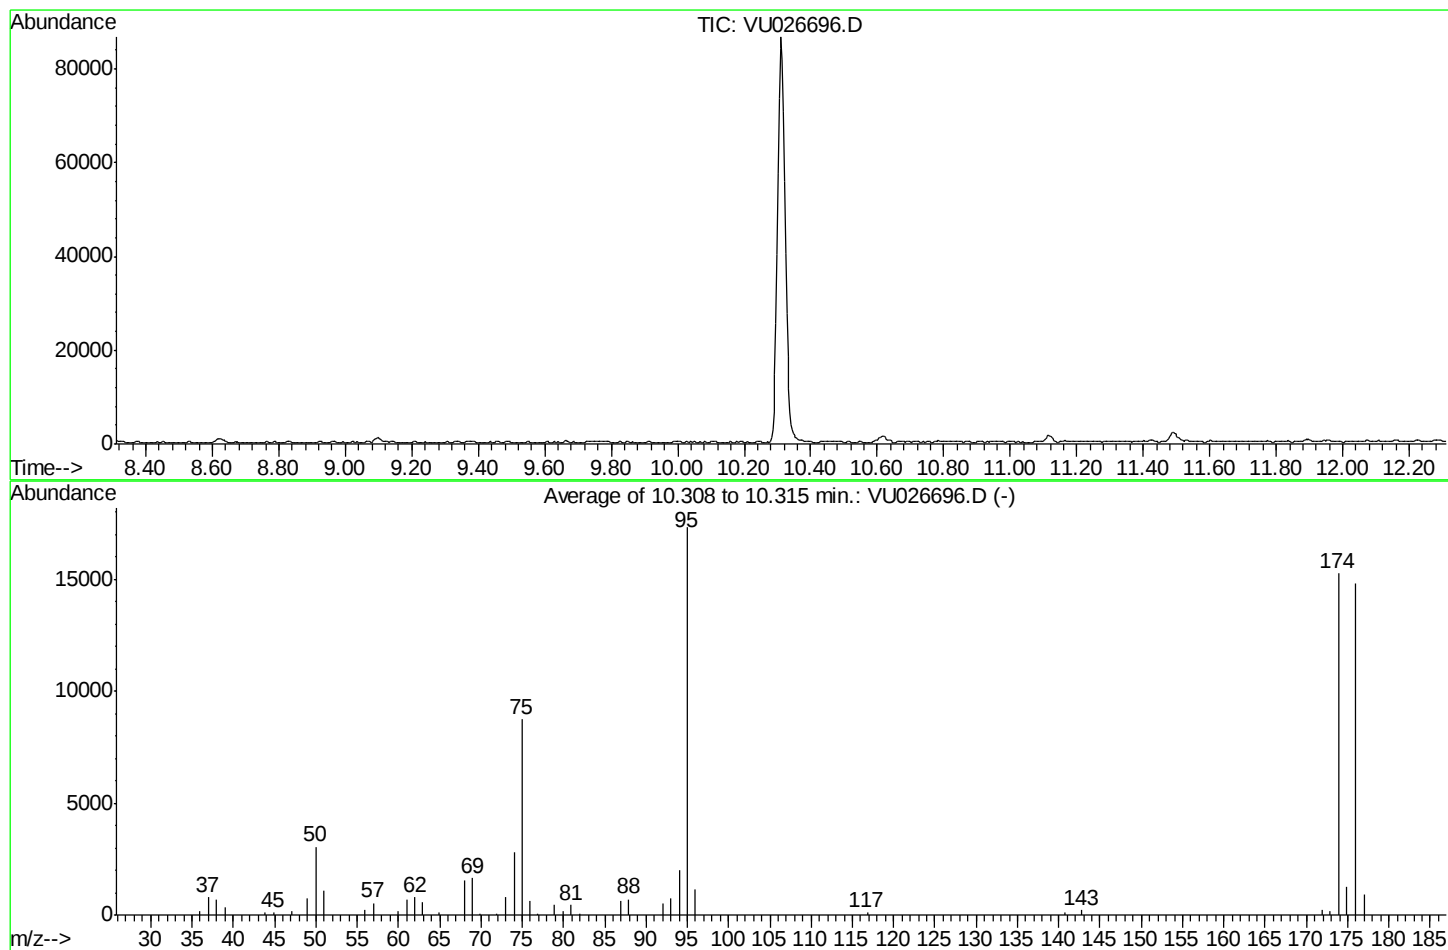

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	3052	PASS
75	95	30	80	50.4	8727	PASS
95	95	100	100	100.0	17309	PASS
96	95	5	9	6.6	1137	PASS
173	174	0.00	2	1.2	190	PASS
174	95	50	120	88.0	15236	PASS
175	174	5	9	8.1	1232	PASS
176	174	95	101	97.1	14800	PASS
177	176	5	9	6.3	925	PASS

m/z	Abundance
43.90	375.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.80	143.0
36.90	781.0
37.90	716.0
39.00	344.0
43.90	479.0
44.90	125.0
47.10	194.0
49.00	783.0
50.00	3113.0
51.00	1044.0
56.00	210.0
57.00	522.0
60.00	161.0
61.00	741.0
62.00	805.0
62.90	576.0
64.90	128.0
67.90	1580.0
69.00	1629.0
69.90	100.0
73.00	830.0
74.00	2830.0
75.00	8714.0
76.00	690.0
76.80	125.0
78.90	500.0
79.90	172.0
80.90	456.0
82.00	103.0
86.90	636.0
87.90	819.0
92.00	569.0
93.00	746.0
94.00	1955.0
95.00	17432.0
96.00	1098.0
116.80	112.0
140.80	151.0
142.80	199.0
171.80	226.0
172.90	186.0
173.90	15054.0
174.90	1186.0
175.90	14374.0
176.90	909.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.00	160.0
37.00	814.0
38.00	721.0
39.00	340.0
43.00	464.0
44.00	105.0
47.10	186.0
49.00	757.0
50.00	3143.0
51.00	1153.0
56.00	230.0
57.00	570.0
60.00	169.0
61.00	736.0
62.00	788.0
62.90	584.0
64.00	148.0
68.00	1553.0
69.00	1695.0
73.00	828.0
74.00	2928.0
75.00	9051.0
76.00	644.0
76.90	116.0
78.90	508.0
79.90	165.0
80.90	465.0
86.90	663.0
87.90	722.0
92.00	567.0
93.00	724.0
94.00	2050.0
95.00	17848.0
96.00	1191.0
116.80	114.0
140.80	149.0
142.80	207.0
171.90	215.0
172.90	203.0
173.90	15652.0
174.90	1287.0
175.90	15218.0
177.00	952.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.00	150.0
37.00	739.0
38.00	679.0
39.00	308.0
43.00	469.0
44.00	102.0
47.00	168.0
49.00	662.0
50.00	2900.0
51.00	1074.0
56.00	219.0
57.00	534.0
59.00	158.0
61.00	655.0
62.00	807.0
62.00	551.0
64.00	150.0
68.00	1458.0
69.00	1615.0
71.00	123.0
73.00	715.0
74.00	2702.0
75.00	8418.0
76.00	570.0
79.00	441.0
79.00	150.0
80.00	422.0
86.00	668.0
87.00	598.0
92.00	473.0
93.00	687.0
94.00	1938.0
95.00	16648.0
96.00	1122.0
116.00	104.0
140.00	131.0
142.00	216.0
171.00	186.0
172.00	183.0
173.00	15002.0
174.00	1223.0
175.00	14809.0
177.00	916.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40