


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091322\
Data File : VU050706.D
Acq On : 13 Sep 2022 15:21
Operator : JC/MD
Sample : BFB124
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB124

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Title : VOC Analysis
Last Update : Wed Sep 14 02:03:10 2022

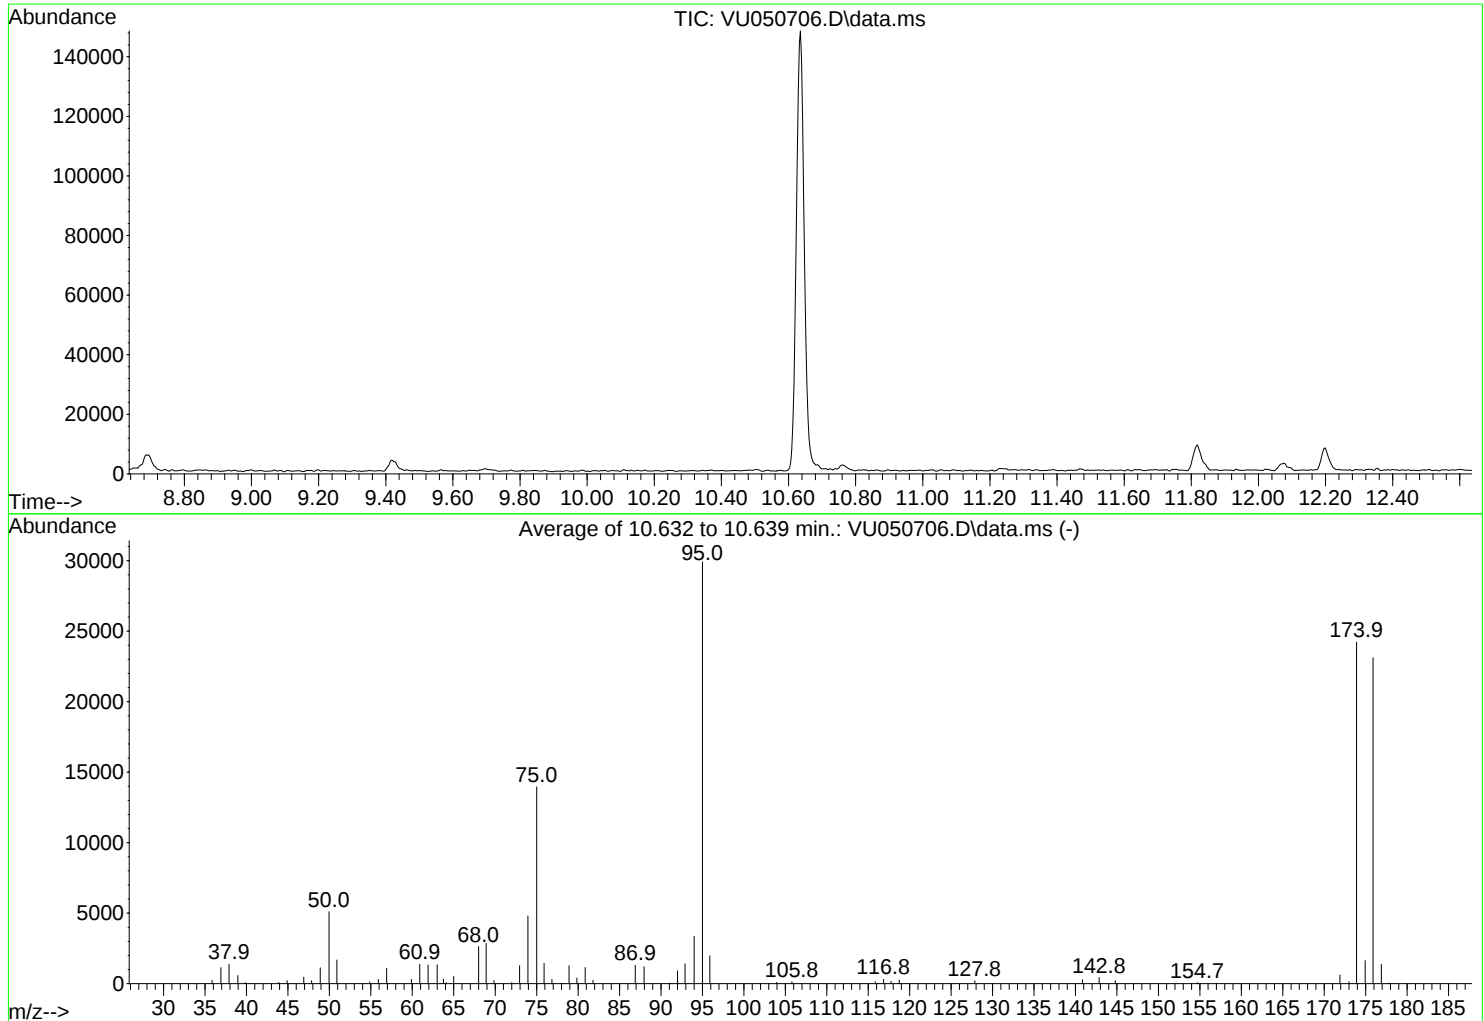

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	5110	PASS
75	95	30	80	46.6	13954	PASS
95	95	100	100	100.0	29917	PASS
96	95	5	9	6.6	1972	PASS
173	174	0.00	2	0.6	138	PASS
174	95	50	120	81.0	24219	PASS
175	174	5	9	6.8	1638	PASS
176	174	95	101	95.5	23123	PASS
177	176	5	9	5.9	1368	PASS

m/z	Abundance
39.80	241.0
43.90	826.0

Instrument :
MSVOA_U
ClientSampleId :
BFB124

m/z	Abundance
35.90	256.0
36.90	1129.0
37.90	1260.0
38.90	522.0
39.90	285.0
43.90	956.0
44.90	225.0
46.90	458.0
47.80	209.0
48.90	1170.0
50.00	5012.0
50.90	1706.0
54.80	104.0
55.90	296.0
56.90	1125.0
59.90	306.0
60.90	1512.0
61.90	1435.0
63.00	1533.0
63.80	359.0
65.00	474.0
68.00	2636.0
68.90	3040.0
69.80	279.0
72.90	1241.0
73.90	4840.0
75.00	14290.0
75.90	1539.0
76.80	311.0
78.90	1450.0
79.80	318.0
80.80	1222.0
81.80	200.0
86.90	1138.0
88.00	1221.0
92.00	916.0
92.90	1443.0
94.00	3361.0
95.00	29768.0
95.90	2071.0
105.80	104.0
115.80	114.0
116.90	322.0
117.70	185.0
118.70	222.0
127.80	201.0
140.90	266.0
142.80	414.0
144.80	219.0
154.70	119.0
171.90	543.0
173.90	24344.0
174.90	1714.0
175.90	23024.0
176.90	1525.0

Instrument :
MSVOA_U
ClientSampleId :
BFB124

m/z	Abundance
35.80	217.0
36.90	1163.0
37.90	1482.0
39.00	598.0
39.90	324.0
43.90	919.0
44.90	222.0
46.90	511.0
47.90	217.0
48.90	1158.0
49.90	5269.0
50.90	1746.0
54.90	120.0
55.90	304.0
56.90	1130.0
59.90	308.0
60.90	1447.0
61.90	1349.0
63.00	1363.0
63.80	342.0
65.00	530.0
68.00	2689.0
68.90	2952.0
69.80	224.0
72.00	124.0
73.00	1324.0
73.90	4942.0
75.00	14160.0
75.90	1485.0
76.80	320.0
78.90	1335.0
79.90	424.0
80.90	1193.0
81.80	232.0
86.90	1362.0
87.90	1204.0
92.00	952.0
92.90	1422.0
94.00	3467.0
95.00	30976.0
95.90	2083.0
103.90	126.0
105.80	165.0
115.90	132.0
116.80	322.0
117.80	175.0
118.70	266.0
127.90	190.0
140.80	276.0
142.80	423.0
144.80	215.0
154.70	102.0
171.90	626.0
173.90	24904.0
175.00	1691.0
175.90	23952.0
176.90	1365.0
177.80	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB124

m/z	Abundance
35.90	230.0
36.90	1109.0
37.90	1367.0
39.00	623.0
40.00	341.0
43.90	867.0
44.90	186.0
46.90	421.0
47.90	181.0
48.90	1055.0
49.90	5050.0
50.90	1602.0
54.90	104.0
55.90	299.0
56.90	970.0
59.90	285.0
60.90	1181.0
61.90	1214.0
63.00	1135.0
63.70	239.0
64.10	227.0
65.00	513.0
68.00	2559.0
68.90	2584.0
69.90	186.0
72.00	104.0
73.00	1263.0
74.00	4630.0
75.00	13411.0
75.90	1307.0
76.90	281.0
78.00	119.0
78.90	1028.0
79.90	437.0
80.90	1013.0
81.80	273.0
86.90	1413.0
87.90	1153.0
91.00	109.0
92.00	852.0
92.90	1374.0
94.00	3242.0
95.00	29008.0
95.90	1761.0
104.00	145.0
105.80	154.0
115.90	160.0
116.80	279.0
117.80	131.0
118.80	269.0
127.90	211.0
140.80	262.0
142.90	471.0
144.80	194.0
171.90	685.0
173.00	414.0
173.90	23408.0
175.00	1508.0
175.90	22392.0
176.90	1213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB124