

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091323\
 Data File : VU055288.D
 Acq On : 13 Sep 2023 16:41
 Operator : MD/SY
 Sample : 04307-04DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4N6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	107	rVB	37049	43938	5.79%	0.754%
2	1.911	185	193	206	rBV	66441	85881	11.32%	1.473%
3	2.564	383	396	412	rBV3	93178	177702	23.42%	3.049%
4	3.043	529	545	560	rVB2	17173	31952	4.21%	0.548%
5	3.181	571	588	607	rBV2	12202	29888	3.94%	0.513%
6	4.631	1025	1039	1080	rBV	105008	367078	48.37%	6.298%
7	5.062	1157	1173	1194	rBV	114000	261612	34.48%	4.489%
8	5.724	1357	1379	1401	rBV3	206131	548014	72.22%	9.402%
9	6.248	1526	1542	1565	rBV	220728	431764	56.90%	7.408%
10	6.541	1616	1633	1652	rBV2	227514	442454	58.31%	7.591%
11	6.689	1667	1679	1698	rBV	141157	281327	37.07%	4.827%
12	7.567	1941	1952	1974	rBV2	50001	91698	12.08%	1.573%
13	7.898	2038	2055	2084	rBV	232614	413373	54.47%	7.092%
14	8.181	2133	2143	2161	rBV2	29739	50491	6.65%	0.866%
15	8.554	2249	2259	2273	rBV4	22301	40341	5.32%	0.692%
16	8.634	2273	2284	2319	rBV4	306314	758845	100.00%	13.020%
17	9.415	2515	2527	2549	rBV	349560	590805	77.86%	10.137%
18	10.753	2930	2943	2960	rBV	116794	191196	25.20%	3.280%
19	11.811	3260	3272	3292	rBV	354832	576722	76.00%	9.895%
20	12.193	3378	3391	3411	rBV	247431	413399	54.48%	7.093%




Sum of corrected areas: 5828480

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091323\
Data File : VU055288.D
Acq On : 13 Sep 2023 16:41
Operator : MD/SY
Sample : 04307-04DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4N6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

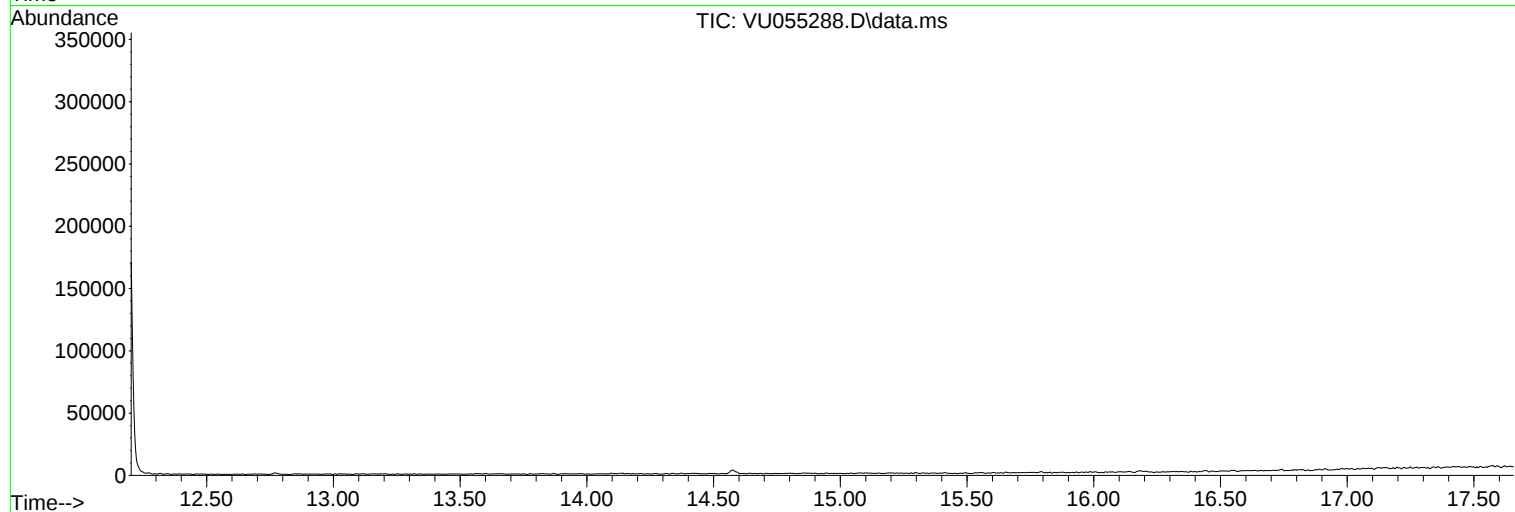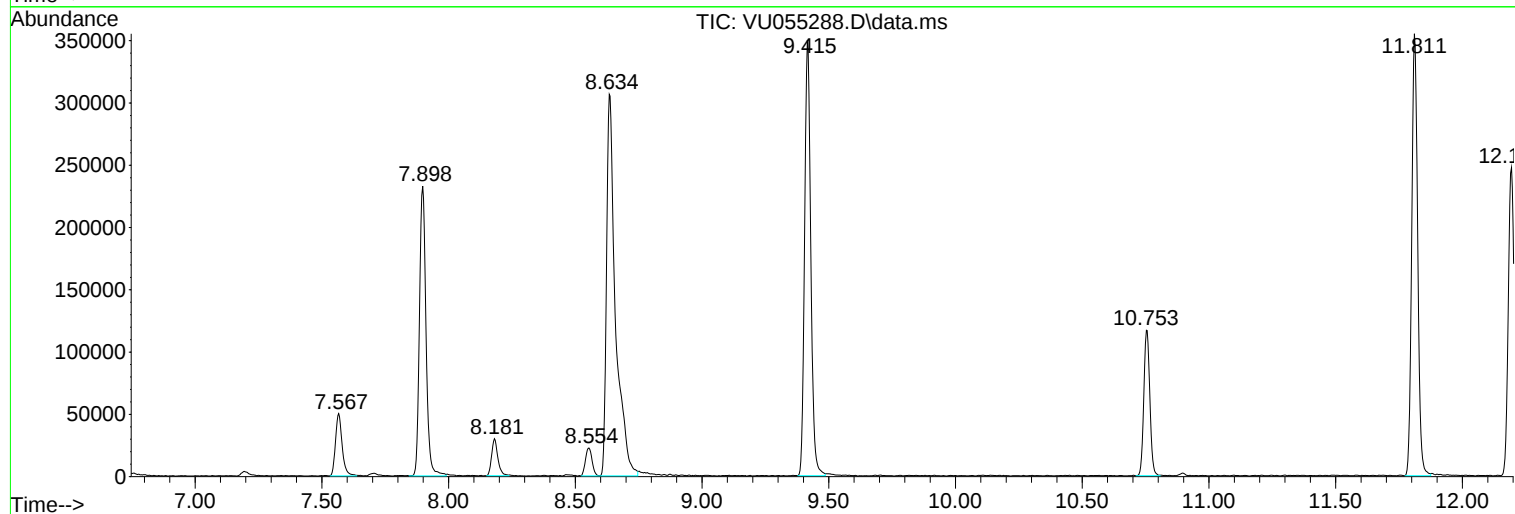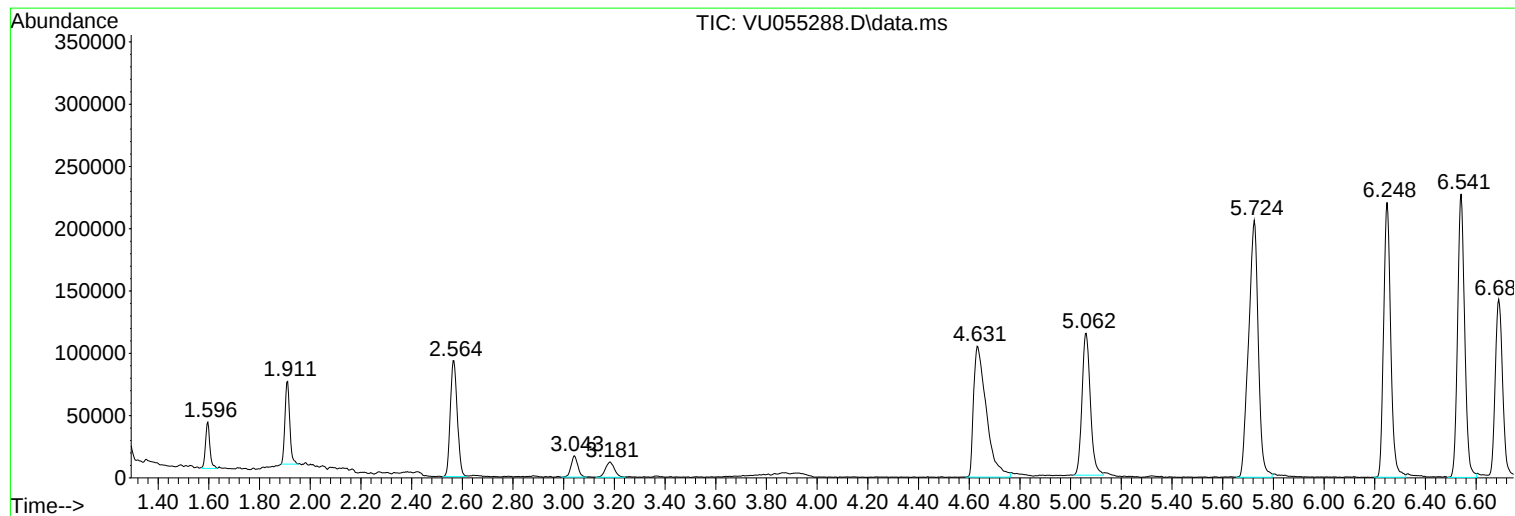

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091323\
Data File : VU055288.D
Acq On : 13 Sep 2023 16:41
Operator : MD/SY
Sample : 04307-04DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4N6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091323\
Data File : VU055288.D
Acq On : 13 Sep 2023 16:41
Operator : MD/SY
Sample : 04307-04DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4N6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc