

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091323\
 Data File : VU055295.D
 Acq On : 13 Sep 2023 19:32
 Operator : MD/SY
 Sample : 04306-09 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4K6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	105	rVB	37707	45477	6.10%	0.769%
2	1.908	185	192	208	rVB	65751	88695	11.90%	1.500%
3	2.563	384	396	410	rBV	77665	127889	17.16%	2.162%
4	3.043	535	545	559	rVB2	12275	22944	3.08%	0.388%
5	3.181	573	588	607	rBV2	33082	78229	10.50%	1.323%
6	3.361	627	644	663	rBV2	130377	309070	41.48%	5.225%
7	4.631	1023	1039	1068	rBV2	126037	401961	53.94%	6.796%
8	5.062	1157	1173	1194	rBV	119235	268674	36.06%	4.542%
9	5.724	1357	1379	1405	rBV2	206784	563557	75.63%	9.528%
10	6.248	1529	1542	1562	rBV2	218375	424325	56.94%	7.174%
11	6.541	1616	1633	1647	rBV3	131661	266640	35.78%	4.508%
12	6.689	1666	1679	1700	rBV	148714	290868	39.03%	4.918%
13	7.566	1940	1952	1966	rBV2	46745	85947	11.53%	1.453%
14	7.898	2042	2055	2071	rBV	228932	400674	53.77%	6.774%
15	8.181	2131	2143	2160	rBV2	27460	50131	6.73%	0.848%
16	8.634	2273	2284	2327	rBV4	298811	745150	100.00%	12.598%
17	9.415	2514	2527	2557	rBV	340389	575246	77.20%	9.726%
18	10.753	2932	2943	2966	rVB	114547	188071	25.24%	3.180%
19	11.811	3260	3272	3292	rBV	349731	570060	76.50%	9.638%
20	12.193	3378	3391	3415	rBV	242195	411125	55.17%	6.951%




Sum of corrected areas: 5914733

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091323\
Data File : VU055295.D
Acq On : 13 Sep 2023 19:32
Operator : MD/SY
Sample : 04306-09 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

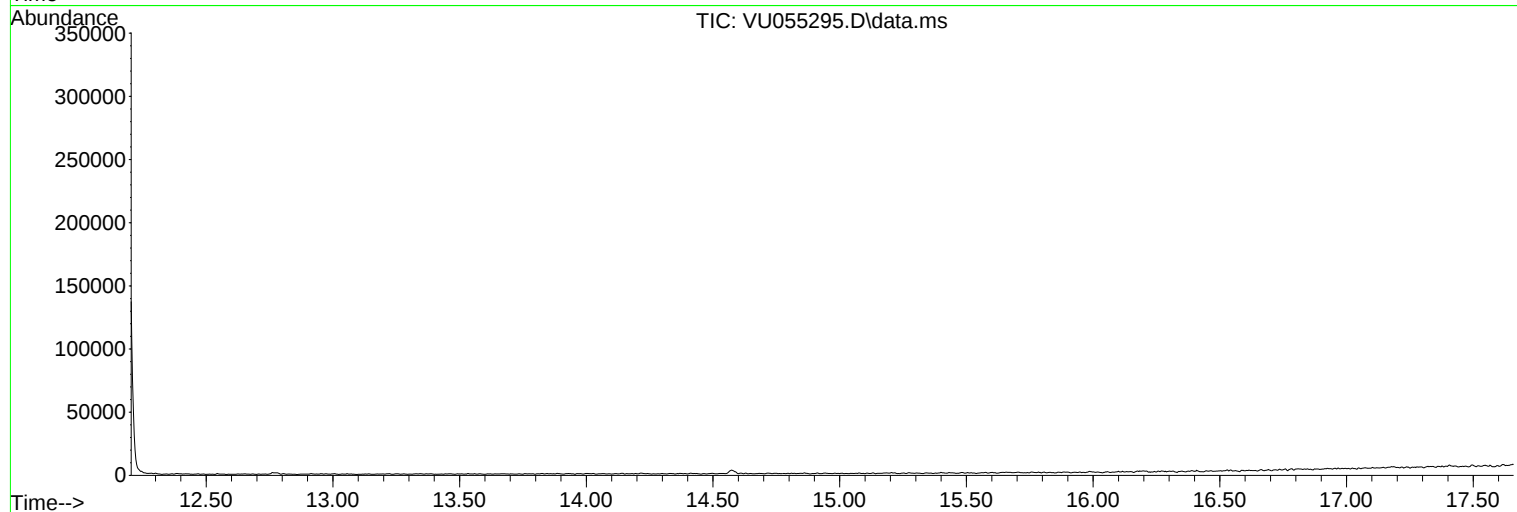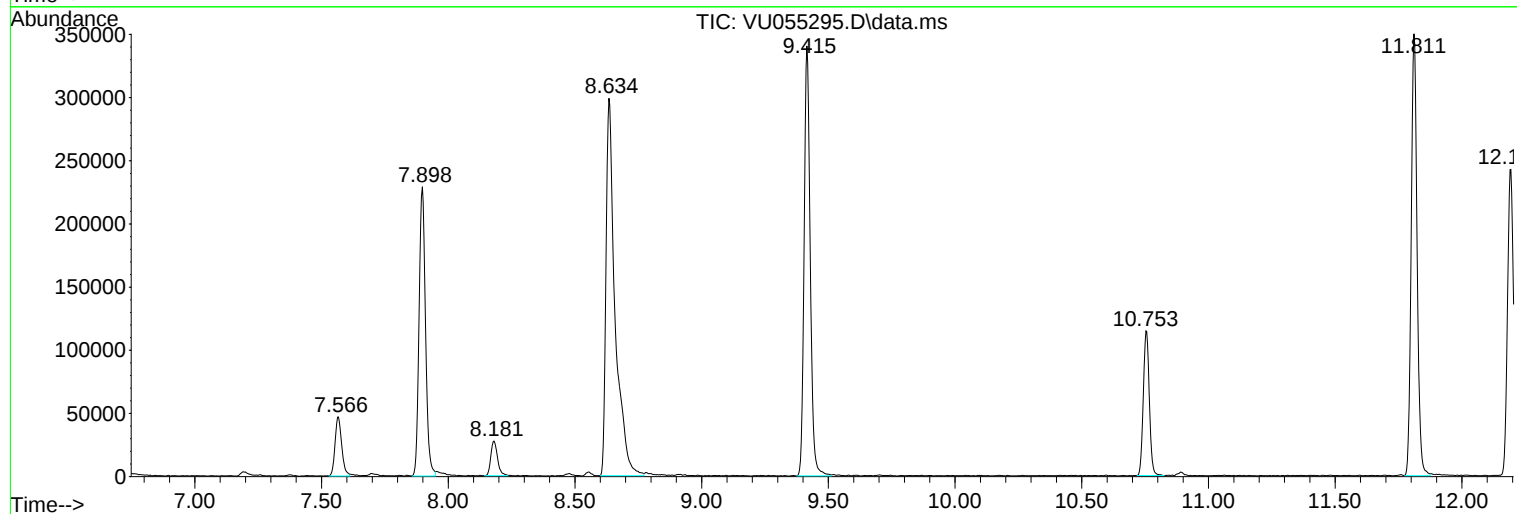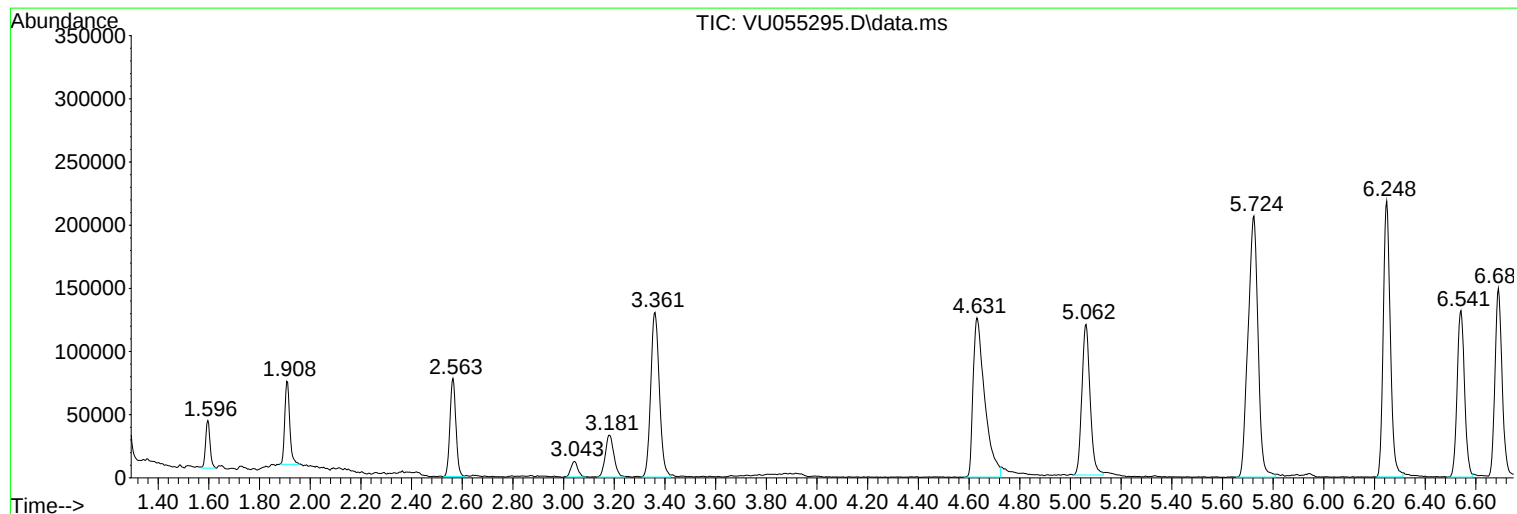

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091323\
Data File : VU055295.D
Acq On : 13 Sep 2023 19:32
Operator : MD/SY
Sample : 04306-09 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091323\
Data File : VU055295.D
Acq On : 13 Sep 2023 19:32
Operator : MD/SY
Sample : 04306-09 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc