


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091323\
Data File : VU055275.D
Acq On : 13 Sep 2023 09:31
Operator : MD/SY
Sample : BFB043
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB043

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Sep 15 02:53:52 2023

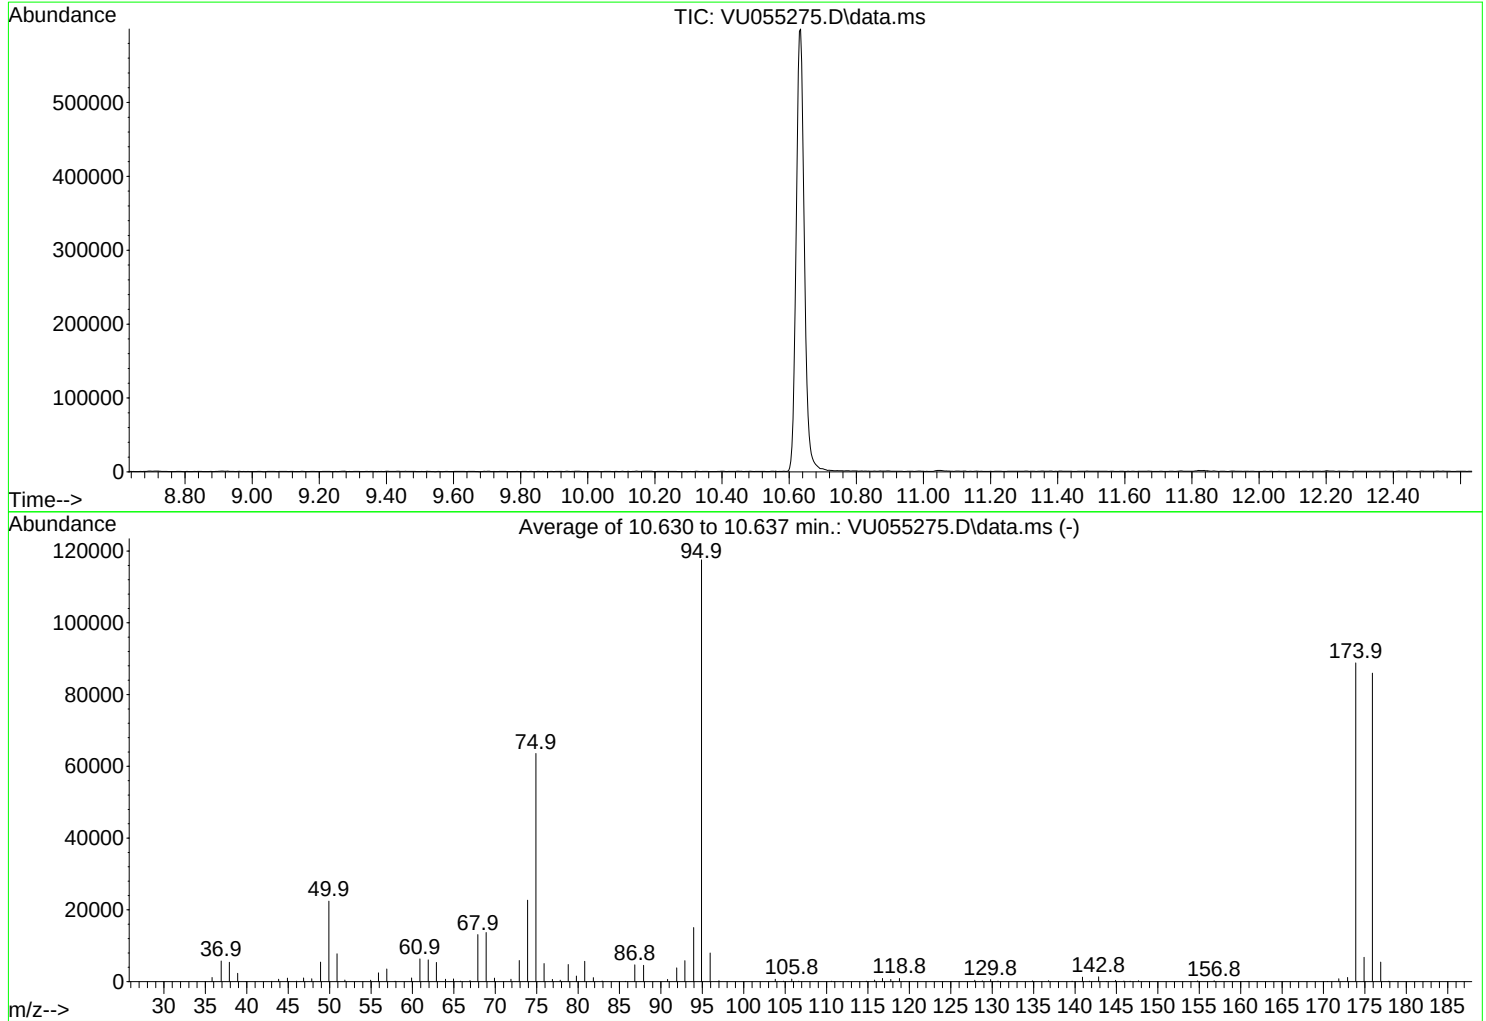

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	22443	PASS
75	95	30	80	54.1	63584	PASS
95	95	100	100	100.0	117549	PASS
96	95	5	9	6.8	7989	PASS
173	174	0.00	2	1.3	1151	PASS
174	95	50	120	75.6	88845	PASS
175	174	5	9	7.6	6768	PASS
176	174	95	101	96.8	85965	PASS
177	176	5	9	6.3	5438	PASS

m/z	Abundance
40.00	185.0
43.90	601.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043

m/z	Abundance
35.80	1294.0
36.90	6158.0
37.90	5489.0
38.90	2504.0
39.80	234.0
43.00	135.0
43.80	1429.0
44.90	976.0
46.00	226.0
46.80	1145.0
47.90	850.0
48.90	5535.0
49.90	24088.0
50.90	7767.0
51.80	517.0
55.00	325.0
55.90	2792.0
56.90	3600.0
57.80	154.0
59.90	1094.0
60.90	6660.0
61.90	6150.0
62.90	4991.0
64.00	620.0
64.90	701.0
65.80	160.0
66.90	356.0
67.90	13721.0
68.90	14100.0
69.90	930.0
71.00	105.0
71.90	740.0
72.90	6391.0
73.90	22920.0
74.90	65712.0
75.90	4938.0
76.90	617.0
77.90	402.0
78.80	4844.0
79.80	1502.0
80.80	5705.0
81.80	1119.0
82.80	191.0
86.90	5032.0
87.90	4754.0
90.80	588.0
91.90	4099.0
92.90	5914.0
94.00	15183.0
94.90	120408.0
96.00	8310.0
97.00	279.0
103.80	826.0
104.80	135.0
105.80	757.0
106.60	140.0
110.60	173.0
114.80	148.0
115.80	544.0
116.70	928.0
117.80	537.0
118.80	883.0
127.90	379.0
128.80	188.0
129.80	572.0
130.70	140.0
134.90	188.0
136.80	267.0
139.70	132.0
140.90	1349.0
141.70	143.0
142.90	1314.0
143.80	109.0
144.90	384.0
145.90	153.0
146.70	119.0
147.60	208.0
154.80	262.0
156.80	273.0
160.90	156.0
170.50	115.0
171.80	733.0
172.90	1081.0
173.90	88792.0
174.90	6869.0
175.90	87304.0
176.90	5566.0
177.90	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043

m/z	Abundance
35.80	1257.0
36.90	5958.0
37.90	5538.0
38.90	2360.0
39.80	217.0
43.00	105.0
43.80	1290.0
44.90	1031.0
46.00	143.0
46.90	1072.0
47.80	829.0
48.90	5626.0
49.90	22832.0
50.90	8034.0
51.90	454.0
55.00	397.0
55.90	2567.0
56.90	3590.0
57.90	146.0
59.90	1035.0
60.90	6554.0
61.90	6193.0
62.90	5582.0
64.00	706.0
65.00	777.0
65.80	148.0
66.90	312.0
67.90	13488.0
68.90	13997.0
69.90	997.0
71.90	702.0
72.90	6066.0
73.90	23344.0
74.90	65040.0
75.90	5233.0
76.90	644.0
77.90	407.0
78.80	4828.0
79.80	1647.0
80.80	5778.0
81.80	1146.0
82.90	173.0
85.70	107.0
86.80	4752.0
87.90	4689.0
90.80	611.0
91.90	3855.0
92.90	6067.0
93.90	15615.0
94.90	120752.0
95.90	8195.0
97.00	302.0
103.80	707.0
104.80	167.0
105.80	701.0
106.70	136.0
110.60	196.0
114.80	164.0
115.80	450.0
116.80	931.0
117.70	648.0
118.80	956.0
127.90	418.0
128.80	252.0
129.80	636.0
130.70	191.0
134.90	243.0
136.80	281.0
139.60	187.0
140.90	1264.0
141.80	171.0
142.90	1359.0
144.90	384.0
145.90	183.0
146.60	149.0
147.70	265.0
154.80	232.0
156.80	258.0
160.90	133.0
171.90	826.0
172.90	1189.0
173.90	91408.0
174.90	7004.0
175.90	88360.0
176.90	5630.0
177.90	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043

m/z	Abundance
35.80	986.0
36.90	5138.0
37.90	5114.0
38.90	2134.0
39.90	176.0
43.90	1096.0
44.90	949.0
46.90	926.0
47.80	753.0
48.90	5221.0
49.90	20408.0
50.90	7440.0
51.90	313.0
54.90	434.0
55.90	1956.0
56.90	3351.0
58.00	133.0
59.90	953.0
60.90	5773.0
61.90	5800.0
62.90	5500.0
64.00	698.0
65.00	790.0
65.80	104.0
67.00	307.0
67.90	12112.0
68.90	13046.0
69.90	1021.0
71.90	577.0
72.90	5208.0
73.90	21776.0
74.90	60000.0
75.90	4954.0
76.90	636.0
77.80	389.0
78.80	4668.0
79.80	1542.0
80.80	5475.0
81.90	1114.0
83.00	149.0
85.70	136.0
86.80	4307.0
87.90	4174.0
90.80	614.0
91.90	3579.0
92.90	5493.0
93.90	14370.0
94.90	111488.0
95.90	7461.0
97.00	293.0
103.80	541.0
104.80	176.0
105.80	651.0
106.70	121.0
110.90	194.0
111.70	116.0
112.60	109.0
114.80	153.0
115.80	364.0
116.80	822.0
117.70	674.0
118.80	897.0
127.90	396.0
128.80	297.0
129.80	555.0
130.70	199.0
134.80	269.0
136.80	281.0
139.60	154.0
140.90	1071.0
141.70	164.0
142.80	1379.0
144.90	285.0
145.90	163.0
146.70	172.0
147.70	286.0
154.80	214.0
156.80	224.0
171.90	816.0
172.90	1182.0
173.90	86336.0
174.90	6430.0
175.90	82232.0
176.90	5118.0
177.90	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043