

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091324\
 Data File : VU060760.D
 Acq On : 13 Sep 2024 17:57
 Operator : MD/SY
 Sample : P3918-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAN1

Quant Time: Sep 14 00:37:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 14 00:33:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	52507	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	84680	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	36729	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	14418	6.217	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	124.400%
7) Chloroethane-d5	1.911	69	16234	4.620	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.400%
11) 1,1-Dichloroethene-d2	2.560	65	7727	5.653	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	113.000%
20) 2-Butanone-d5	4.634	46	30072	37.708	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.420%
24) Chloroform-d	5.055	84	33182	5.019	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
26) 1,2-Dichloroethane-d4	5.698	65	17986	5.213	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.200%
32) Benzene-d6	5.721	84	51815	2.798	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	56.000%#
36) 1,2-Dichloropropane-d6	6.682	67	32294	5.405	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.200%
41) Toluene-d8	7.891	98	81795	4.708	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.200%
43) trans-1,3-Dichloroprop...	8.177	79	10147	4.746	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.000%
46) 2-Hexanone-d5	8.628	63	39136	38.234	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.460%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	25747	4.843	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.800%
66) 1,2-Dichlorobenzene-d4	12.187	152	30617	5.653	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.000%
Target Compounds						
					Qvalue	
13) Acetone	2.653	43	9519	14.264	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091324\
Data File : VU060760.D
Acq On : 13 Sep 2024 17:57
Operator : MD/SY
Sample : P3918-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN1

Quant Time: Sep 14 00:37:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 14 00:33:41 2024
Response via : Initial Calibration

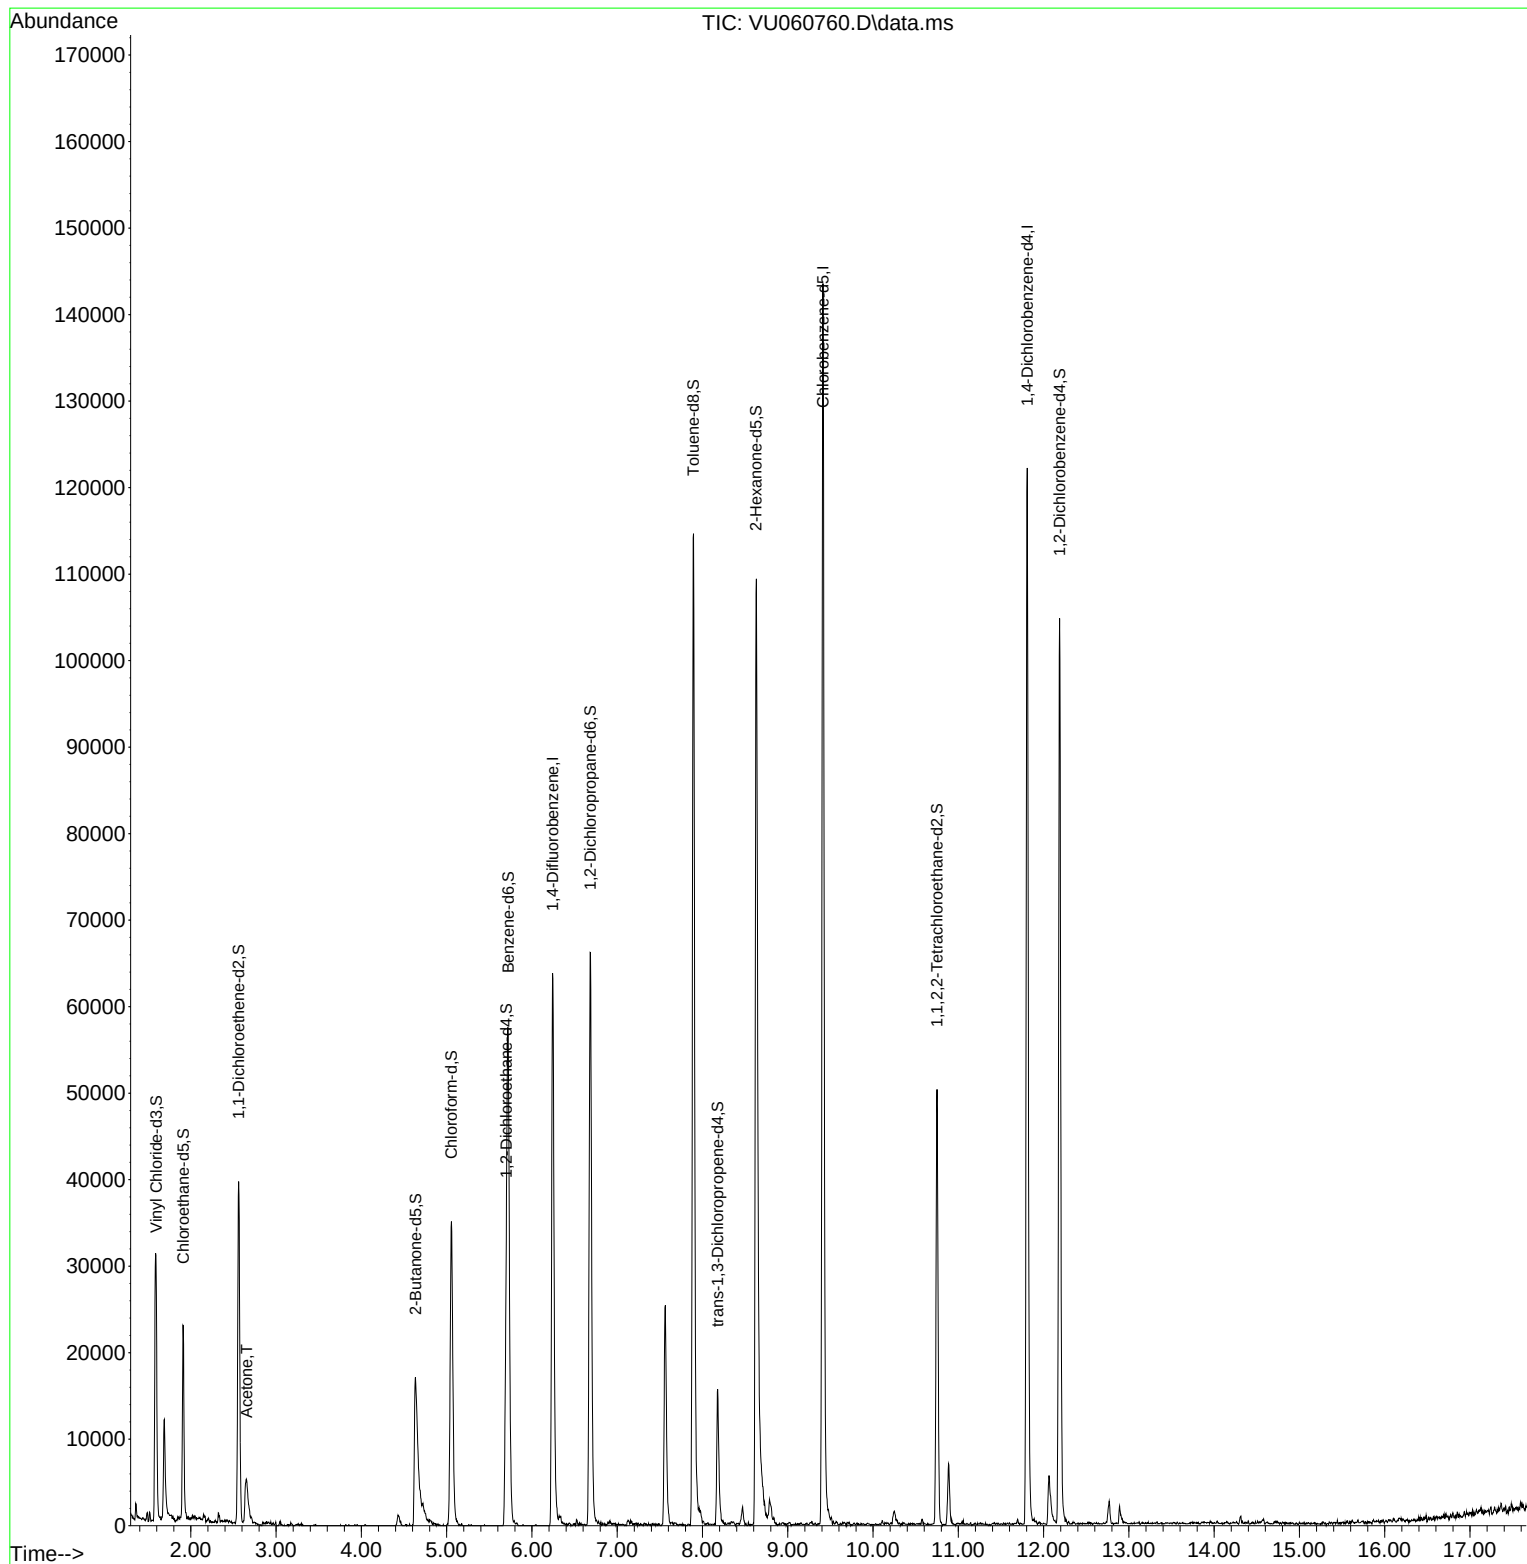

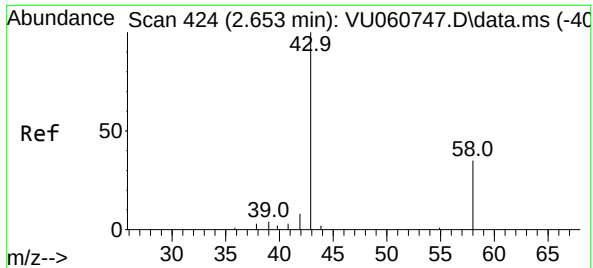

#13
 Acetone
 Concen: 14.264 ug/L
 RT: 2.653 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VU060760.D
 Acq: 13 Sep 2024 17:57

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN1

Tgt Ion: 43 Resp: 9519
 Ion Ratio Lower Upper
 43 100
 58 31.1 0.0 66.8

