


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091324\
Data File : VU060746.D
Acq On : 13 Sep 2024 10:54
Operator : MD/SY
Sample : BFB196
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB196

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Sep 14 00:33:41 2024

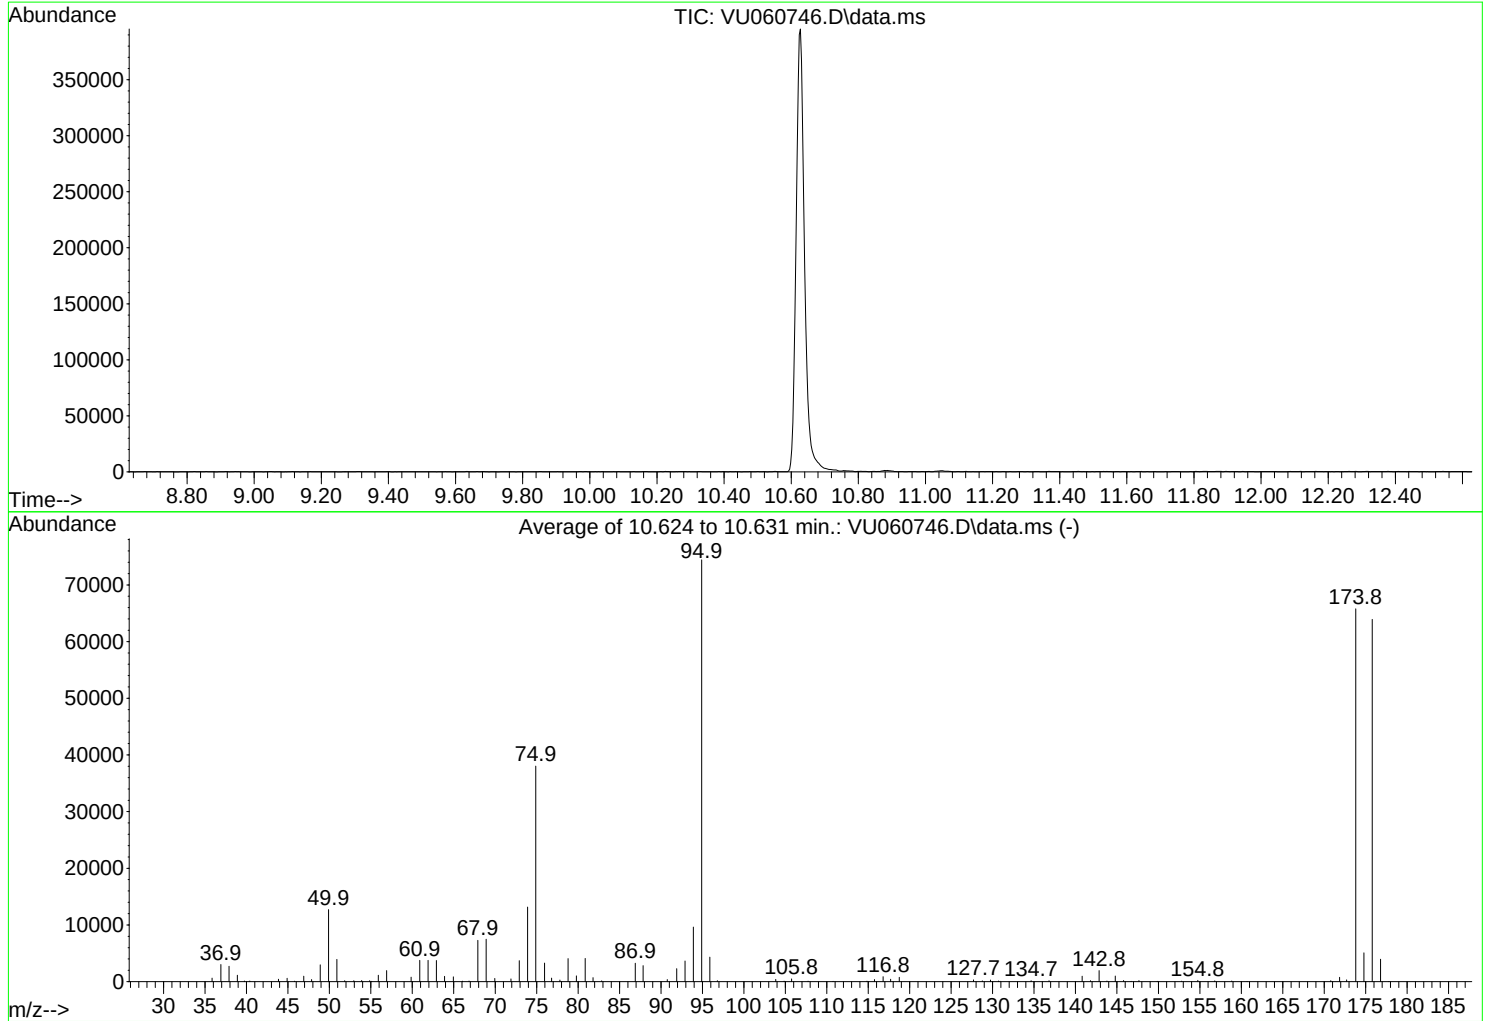

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	12703	PASS
75	95	30	80	51.1	38037	PASS
95	95	100	100	100.0	74424	PASS
96	95	5	9	5.8	4320	PASS
173	174	0.00	2	0.5	325	PASS
174	95	50	120	88.4	65781	PASS
175	174	5	9	7.7	5083	PASS
176	174	95	101	97.2	63928	PASS
177	176	5	9	6.2	3946	PASS

m/z	Abundance
43.80	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB196

m/z	Abundance
35.90	752.0
36.90	3014.0
37.90	2876.0
38.90	1395.0
40.40	183.0
44.00	650.0
44.90	576.0
46.90	1053.0
48.00	350.0
48.90	3064.0
49.90	13130.0
50.90	4262.0
51.90	173.0
53.00	161.0
53.90	223.0
54.80	294.0
55.90	1129.0
56.90	1951.0
59.80	809.0
60.90	3942.0
61.90	3860.0
62.90	3737.0
63.90	894.0
65.00	906.0
66.80	116.0
67.90	7427.0
68.90	7704.0
69.90	552.0
71.90	533.0
72.90	3708.0
73.90	13166.0
74.90	39344.0
75.90	3487.0
76.80	566.0
77.80	222.0
78.80	4139.0
79.80	1096.0
80.90	4112.0
81.80	761.0
82.90	123.0
86.90	3115.0
87.80	2855.0
90.70	333.0
91.90	2484.0
92.90	3734.0
93.90	9882.0
94.90	75104.0
95.90	4342.0
96.80	205.0
103.90	422.0
104.80	139.0
105.80	591.0
110.80	107.0
115.80	384.0
116.80	828.0
117.70	397.0
118.80	760.0
127.70	286.0
128.70	114.0
129.80	266.0
130.70	167.0
134.70	187.0
136.80	177.0
140.90	1025.0
141.80	171.0
142.90	1787.0
143.80	140.0
144.80	1014.0
145.80	201.0
146.70	132.0
147.60	183.0
149.90	103.0
154.70	156.0
156.80	126.0
158.80	105.0
160.70	119.0
170.80	304.0
171.90	724.0
172.70	975.0
173.80	66024.0
174.80	5473.0
175.80	63744.0
176.80	4085.0
177.80	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB196

m/z	Abundance
35.80	619.0
36.90	3118.0
37.90	2753.0
38.90	1159.0
39.70	151.0
40.40	156.0
43.90	634.0
44.90	596.0
45.80	105.0
46.90	981.0
47.80	375.0
48.90	3045.0
49.90	13106.0
50.90	4015.0
51.80	188.0
53.00	191.0
53.90	189.0
54.90	229.0
55.90	1160.0
56.90	2010.0
59.80	821.0
60.90	3837.0
61.90	3862.0
62.90	3811.0
63.90	943.0
64.90	836.0
66.00	116.0
66.90	118.0
67.90	7443.0
68.90	7734.0
69.90	556.0
71.90	508.0
72.90	3865.0
73.90	13520.0
74.90	38960.0
75.90	3407.0
76.80	650.0
77.80	298.0
78.80	4154.0
79.80	1077.0
80.90	4181.0
81.80	723.0
82.90	152.0
86.90	3387.0
87.90	2911.0
90.70	377.0
91.90	2340.0
92.90	3736.0
93.90	9894.0
94.90	76864.0
95.90	4453.0
96.80	186.0
103.80	401.0
104.90	112.0
105.80	488.0
107.80	106.0
110.70	105.0
114.90	115.0
115.80	384.0
116.80	925.0
117.70	441.0
118.80	775.0
127.70	327.0
128.70	124.0
129.70	289.0
130.70	156.0
134.60	161.0
136.80	191.0
140.80	1009.0
141.80	168.0
142.90	2039.0
143.80	121.0
144.80	1047.0
145.80	233.0
147.70	204.0
149.80	103.0
152.80	120.0
154.80	226.0
156.80	146.0
158.80	127.0
170.80	240.0
171.90	786.0
173.80	68040.0
174.80	5183.0
175.80	65816.0
176.80	3998.0

Instrument :
MSVOA_U
ClientSampleId :
BFB196

m/z	Abundance
35.80	468.0
36.90	2929.0
37.90	2547.0
38.90	881.0
39.80	176.0
43.80	550.0
44.90	575.0
45.80	121.0
46.90	838.0
47.80	398.0
48.90	2771.0
49.90	11872.0
50.90	3535.0
51.90	176.0
52.90	172.0
53.90	159.0
55.10	187.0
55.90	1120.0
56.90	1913.0
59.90	746.0
60.90	3471.0
61.90	3590.0
62.90	3639.0
63.90	959.0
64.90	781.0
66.10	123.0
66.90	130.0
67.90	7027.0
68.90	7052.0
70.00	573.0
71.90	386.0
72.90	3510.0
73.90	12812.0
74.90	35808.0
76.00	2973.0
76.80	608.0
77.80	311.0
78.80	3941.0
79.80	916.0
80.80	3998.0
81.80	672.0
82.80	145.0
86.90	3219.0
87.90	2674.0
90.80	411.0
91.90	2032.0
92.90	3432.0
93.90	9074.0
94.90	71304.0
95.90	4165.0
96.80	144.0
103.80	379.0
105.70	405.0
107.70	152.0
114.80	171.0
115.70	346.0
116.80	879.0
117.70	403.0
118.70	739.0
127.70	352.0
128.80	150.0
129.70	261.0
130.90	150.0
134.70	136.0
136.80	172.0
140.70	872.0
141.80	151.0
142.80	2014.0
143.80	112.0
144.80	917.0
145.80	193.0
147.70	212.0
152.80	107.0
154.80	299.0
156.80	156.0
158.90	129.0
171.80	820.0
173.80	63280.0
174.80	4592.0
175.80	62224.0
176.80	3756.0

Instrument :
MSVOA_U
ClientSampleId :
BFB196