


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091418\
 Data File : VU026720.D
 Acq On : 13 Sep 2018 08:11
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
 Title : SW846 8260
 Last Update : Wed Sep 12 05:32:45 2018

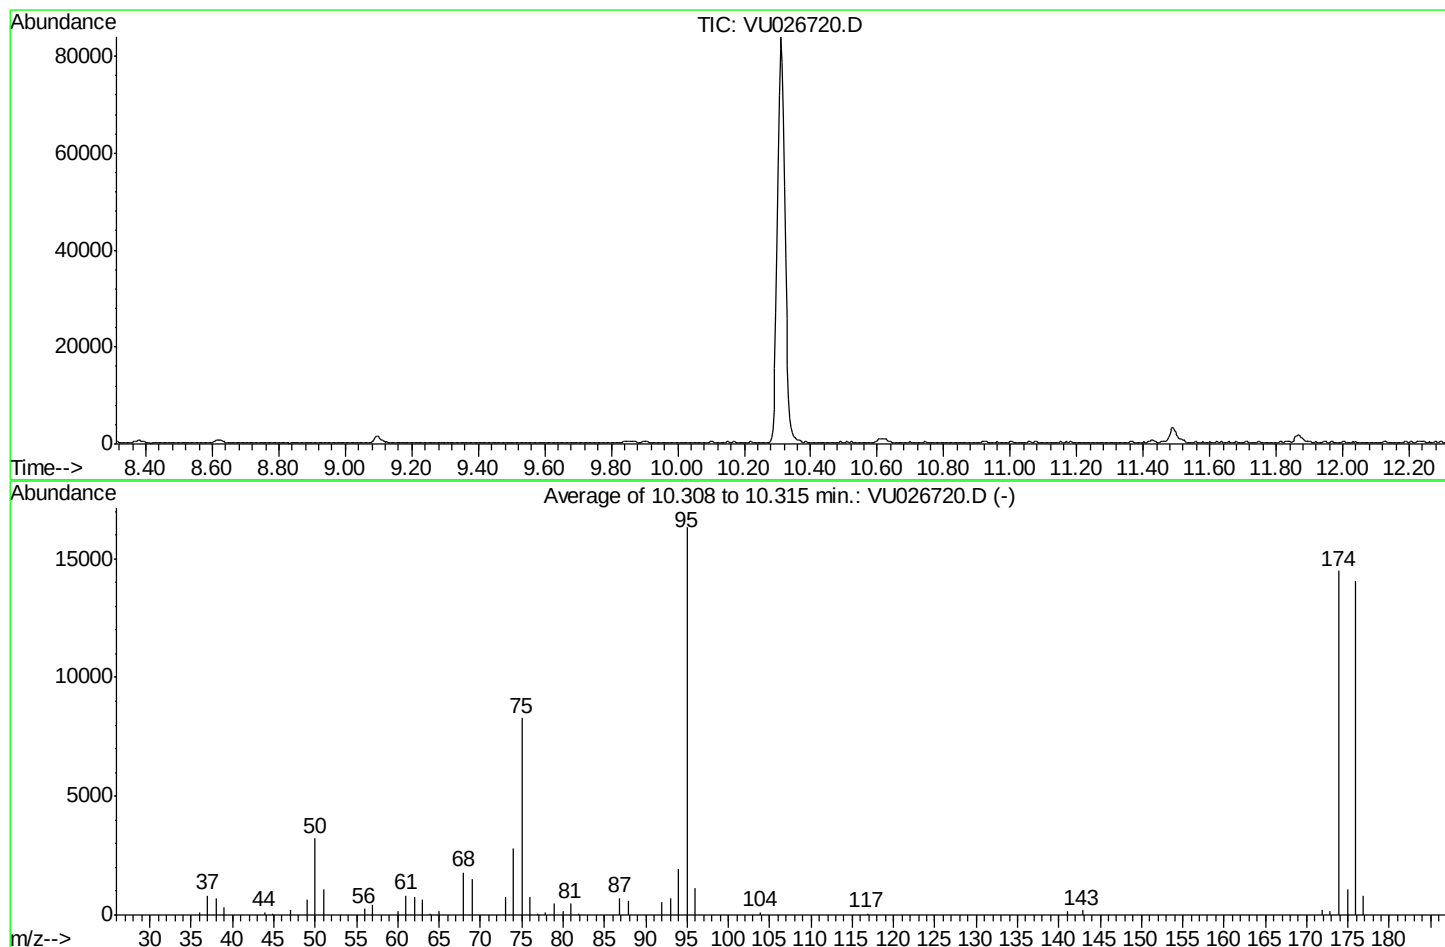

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	3211	PASS
75	95	30	60	50.8	8295	PASS
95	95	100	100	100.0	16321	PASS
96	95	5	9	6.9	1121	PASS
173	174	0.00	2	1.1	157	PASS
174	95	50	100	88.8	14492	PASS
175	174	5	9	7.6	1098	PASS
176	174	95	101	97.2	14085	PASS
177	176	5	9	5.8	812	PASS