


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091420\
Data File : VU040123.D
Acq On : 14 Sep 2020 16:25
Operator : SY/MD
Sample : L3950-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFWT1

Manual Integrations
APPROVED

MMDadoda
9/15/2020 8:30:23 AM

Quant Time: Sep 14 17:08:02 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Sep 14 12:19:40 2020
Response via : Initial Calibration

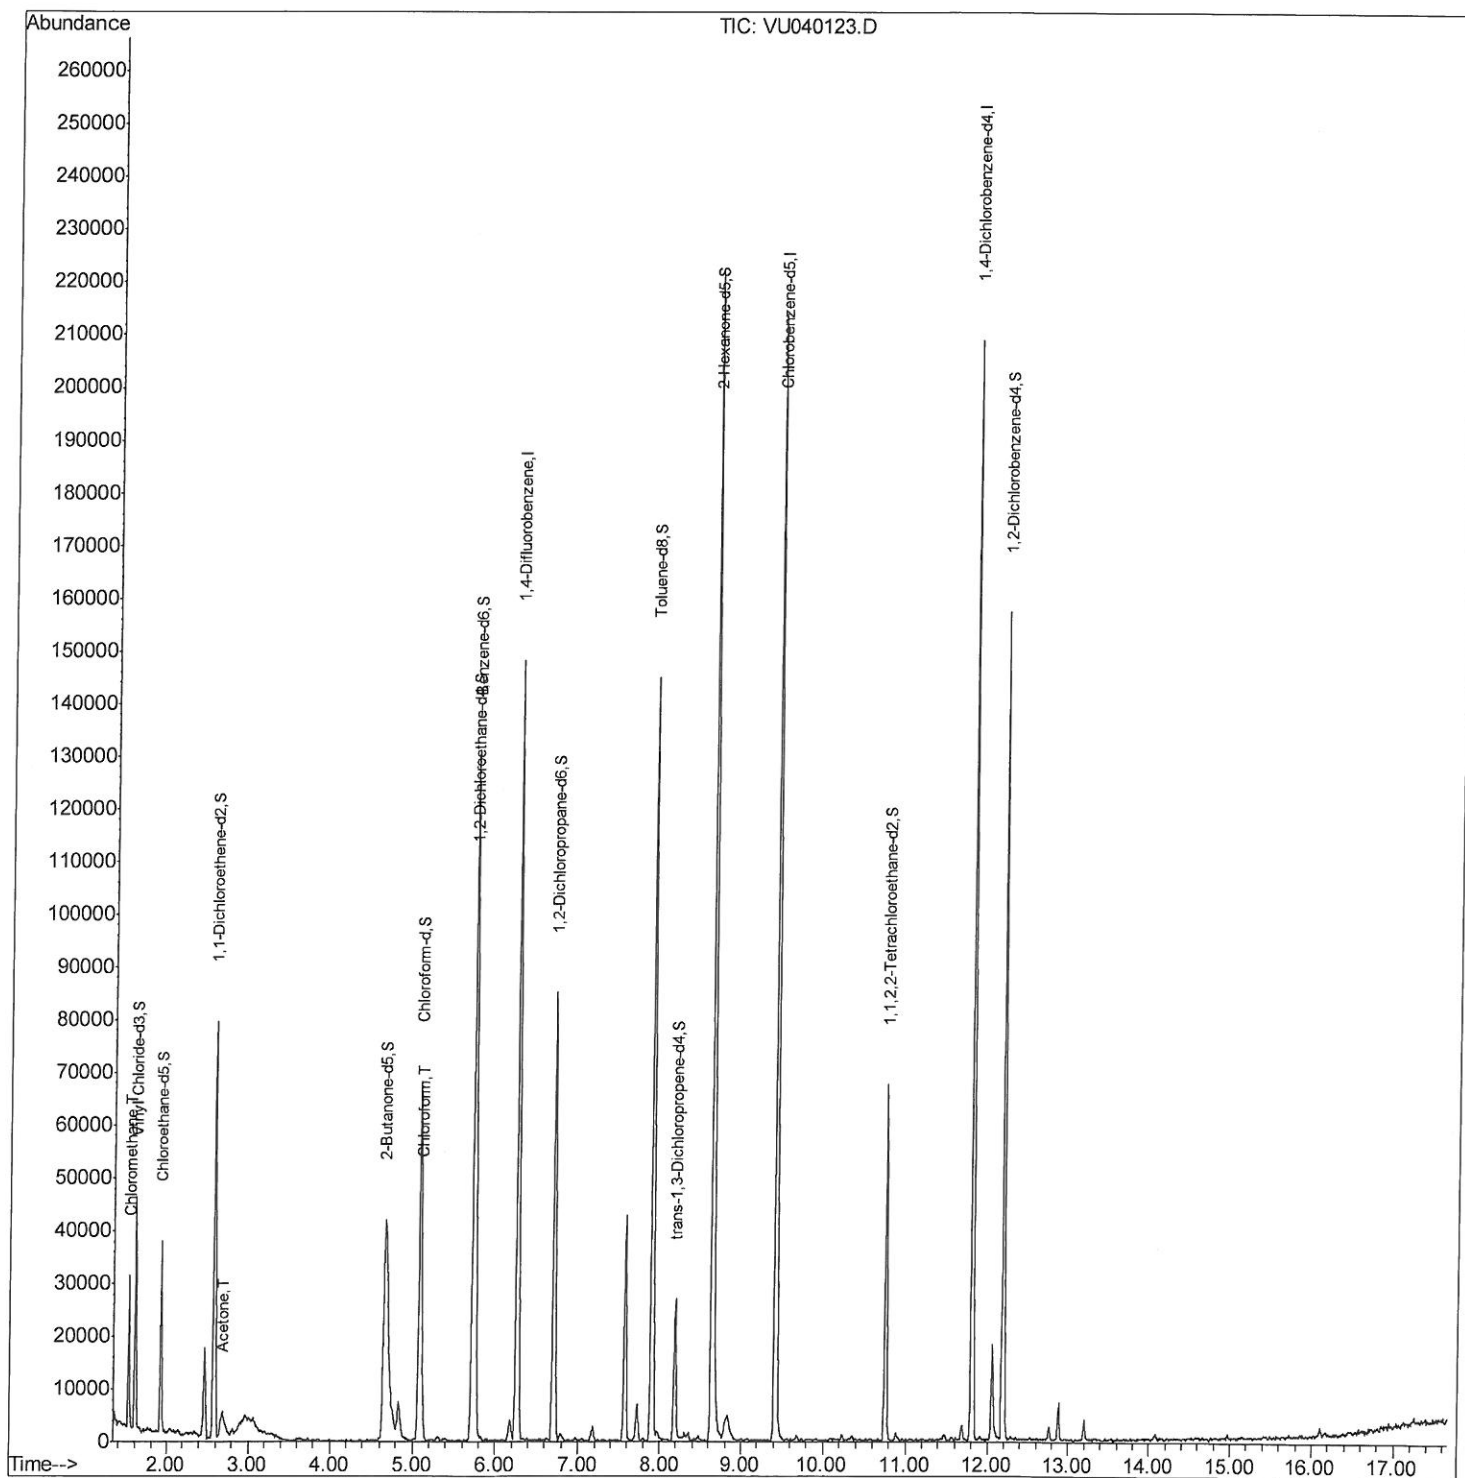

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091420\
Data File : VU040123.D
Acq On : 14 Sep 2020 16:25
Operator : SY/MD
Sample : L3950-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFWT1

Manual Integrations
APPROVED

MMDadoda
9/15/2020 8:30:23 AM

Quant Time: Sep 14 16:57:34 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Sep 14 12:19:40 2020
Response via : Initial Calibration

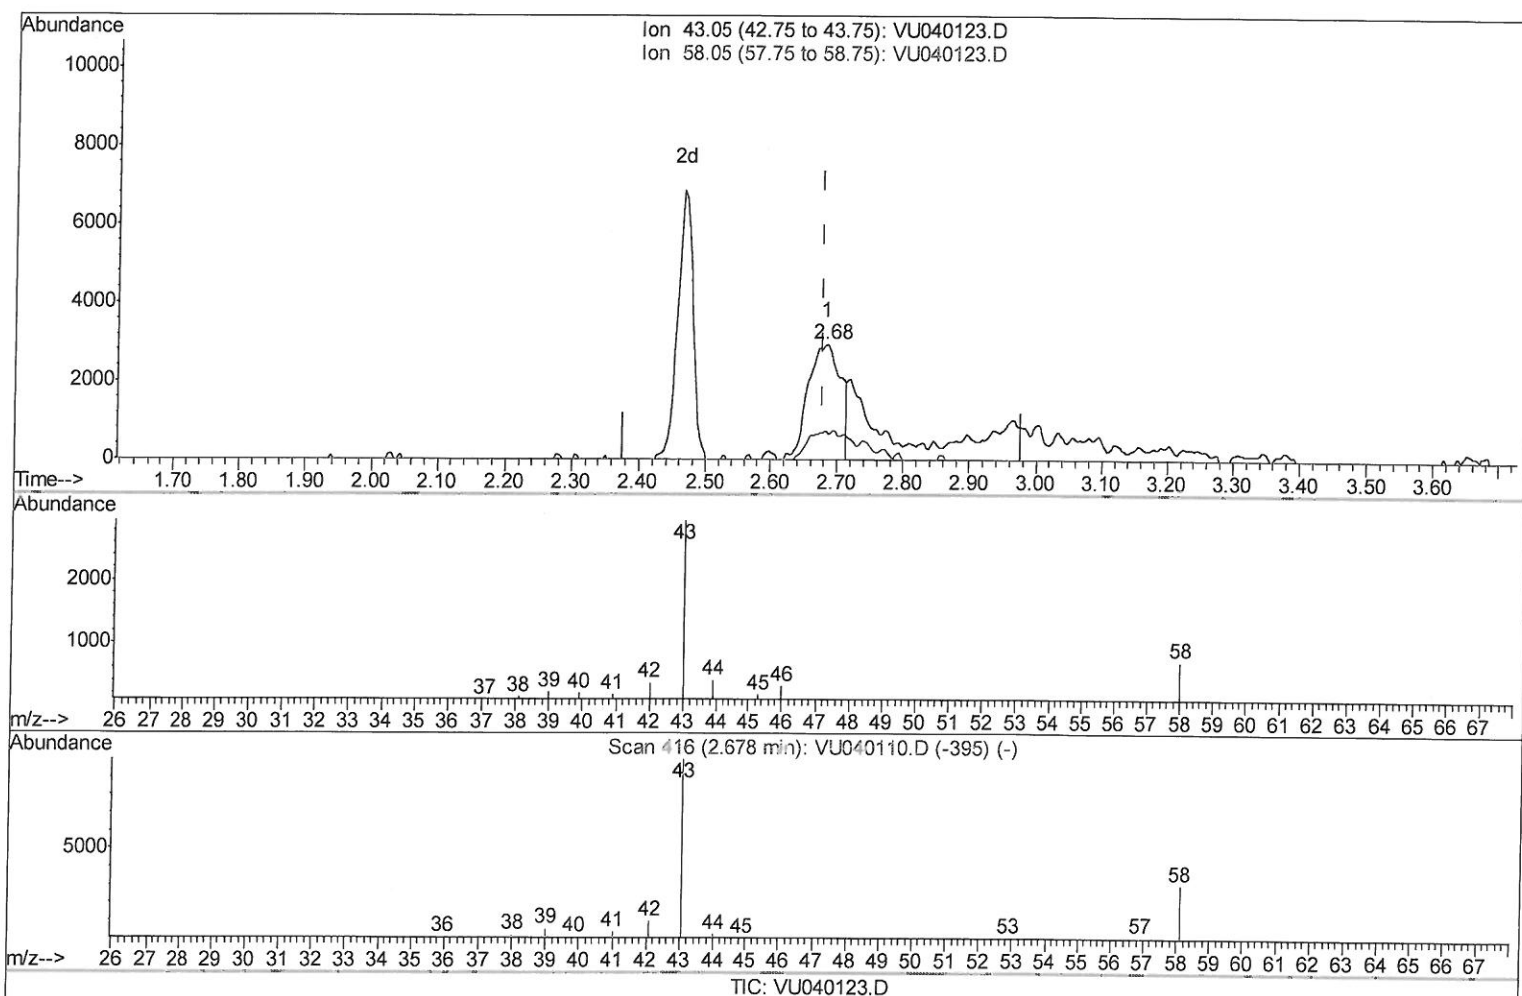

(13) Acetone (T)

2.684min (+0.006) 4.63ug/L

response 9956

Ion	Exp%	Act%
43.05	100	100
58.05	27.70	15.64
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091420\
Data File : VU040123.D
Acq On : 14 Sep 2020 16:25
Operator : SY/MD
Sample : L3950-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFWT1

Manual Integrations
APPROVED

MMDadoda
9/15/2020 8:30:23 AM

Quant Time: Sep 14 16:57:34 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Sep 14 12:19:40 2020
Response via : Initial Calibration

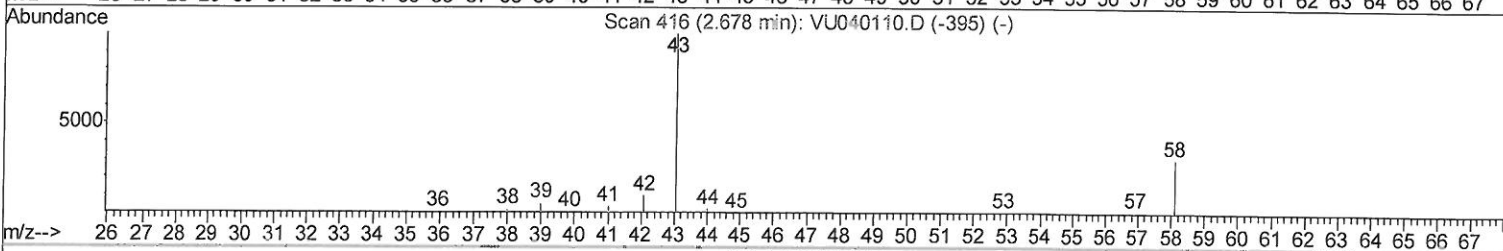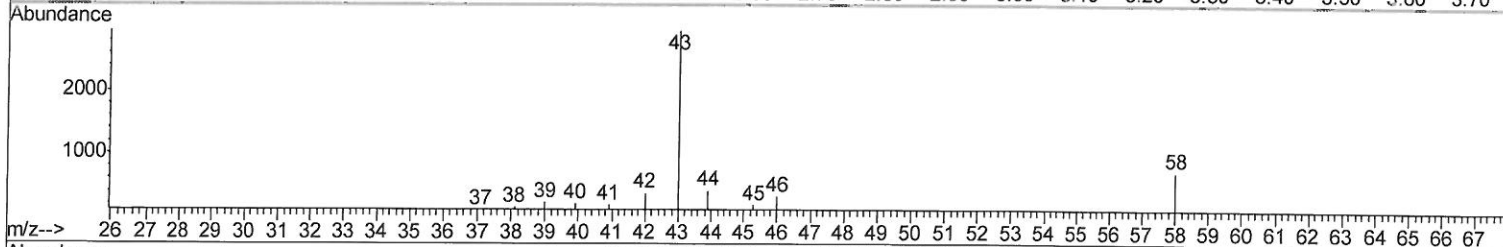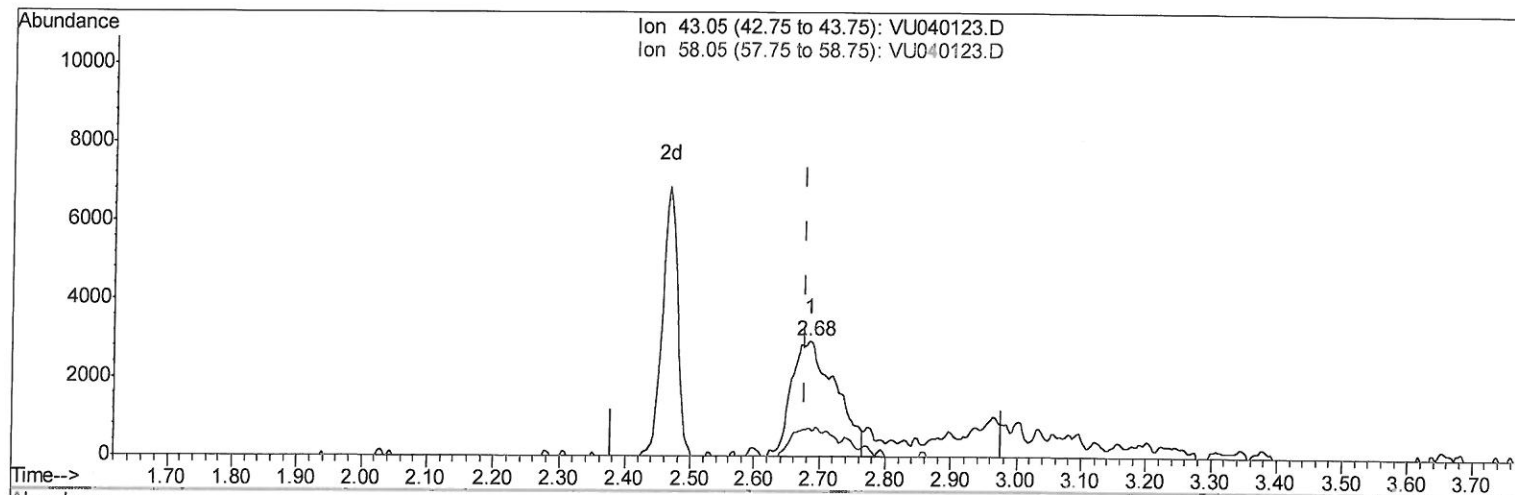

TIC: VU040123.D

(13) Acetone (T)

2.684min (+0.006) 6.50ug/L m

response 13965

Ion	Exp%	Act%
43.05	100	100
58.05	27.70	11.15
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
09/15/20

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091420\
 Data File : VU040123.D
 Acq On : 14 Sep 2020 16:25
 Operator : SY/MD
 Sample : L3950-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 BFWT1

Manual Integrations
 APPROVED

MMDadoda
 9/15/2020 8:30:23 AM

Quant Time: Sep 14 17:08:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Sep 14 12:19:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	106309	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	105623	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	47570	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.60	65	27438	4.73	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	94.60%		
7) Chloroethane-d5	1.92	69	24726	5.11	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	102.20%		
11) 1,1-Dichloroethene-d2	2.58	63	48191	3.24	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	64.80%		
20) 2-Butanone-d5	4.66	46	104407	44.97	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	89.94%		
24) Chloroform-d	5.08	84	59083	4.36	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	87.20%		
26) 1,2-Dichloroethane-d4	5.72	65	35910	4.29	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	85.80%		
32) Benzene-d6	5.74	84	109395	4.44	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	88.80%		
36) 1,2-Dichloropropane-d6	6.70	67	36491	4.49	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	89.80%		
41) Toluene-d8	7.91	98	88770	3.98	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	79.60%		
43) trans-1,3-Dichloropropene-	8.19	79	14323	3.84	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	76.80%		
46) 2-Hexanone-d5	8.64	63	73678	41.66	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	83.32%		
57) 1,1,2,2-Tetrachloroethane-	10.75	84	30584	4.35	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	87.00%		
64) 1,2-Dichlorobenzene-d4	12.19	152	34555	4.49	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	89.80%		
Target Compounds						
3) Chloromethane	1.53	50	18478	1.829	ug/L	97
13) Acetone	2.68	43	13965m	6.498	ug/L	97
25) Chloroform	5.11	83	7495	0.402	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed