

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091420\
 Data File : VU040126.D
 Acq On : 14 Sep 2020 18:21
 Operator : SY/MD
 Sample : L4001-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETYP0

Quant Time: Sep 15 03:27:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 15 01:48:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	103559	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	105274	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	44338	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	30825	5.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.00%
7) Chloroethane-d5	1.92	69	27014	5.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	114.60%
11) 1,1-Dichloroethene-d2	2.58	63	50231	3.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.20%
20) 2-Butanone-d5	4.66	46	111017	49.09	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.18%
24) Chloroform-d	5.08	84	64138	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
26) 1,2-Dichloroethane-d4	5.72	65	39351	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.74	84	117894	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
36) 1,2-Dichloropropane-d6	6.70	67	38565	4.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.20%
41) Toluene-d8	7.91	98	95152	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.80%
43) trans-1,3-Dichloropropene-	8.19	79	14176	3.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.20%
46) 2-Hexanone-d5	8.64	63	77733	44.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.20%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	33933	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.80%
64) 1,2-Dichlorobenzene-d4	12.19	152	37943	5.29	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.80%


Target Compounds					Ovalue
42) Toluene	7.98	91	39272	1.013 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091420\
Data File : VU040126.D
Acq On : 14 Sep 2020 18:21
Operator : SY/MD
Sample : L4001-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETYP0

Quant Time: Sep 15 03:27:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 15 01:48:35 2020
Response via : Initial Calibration

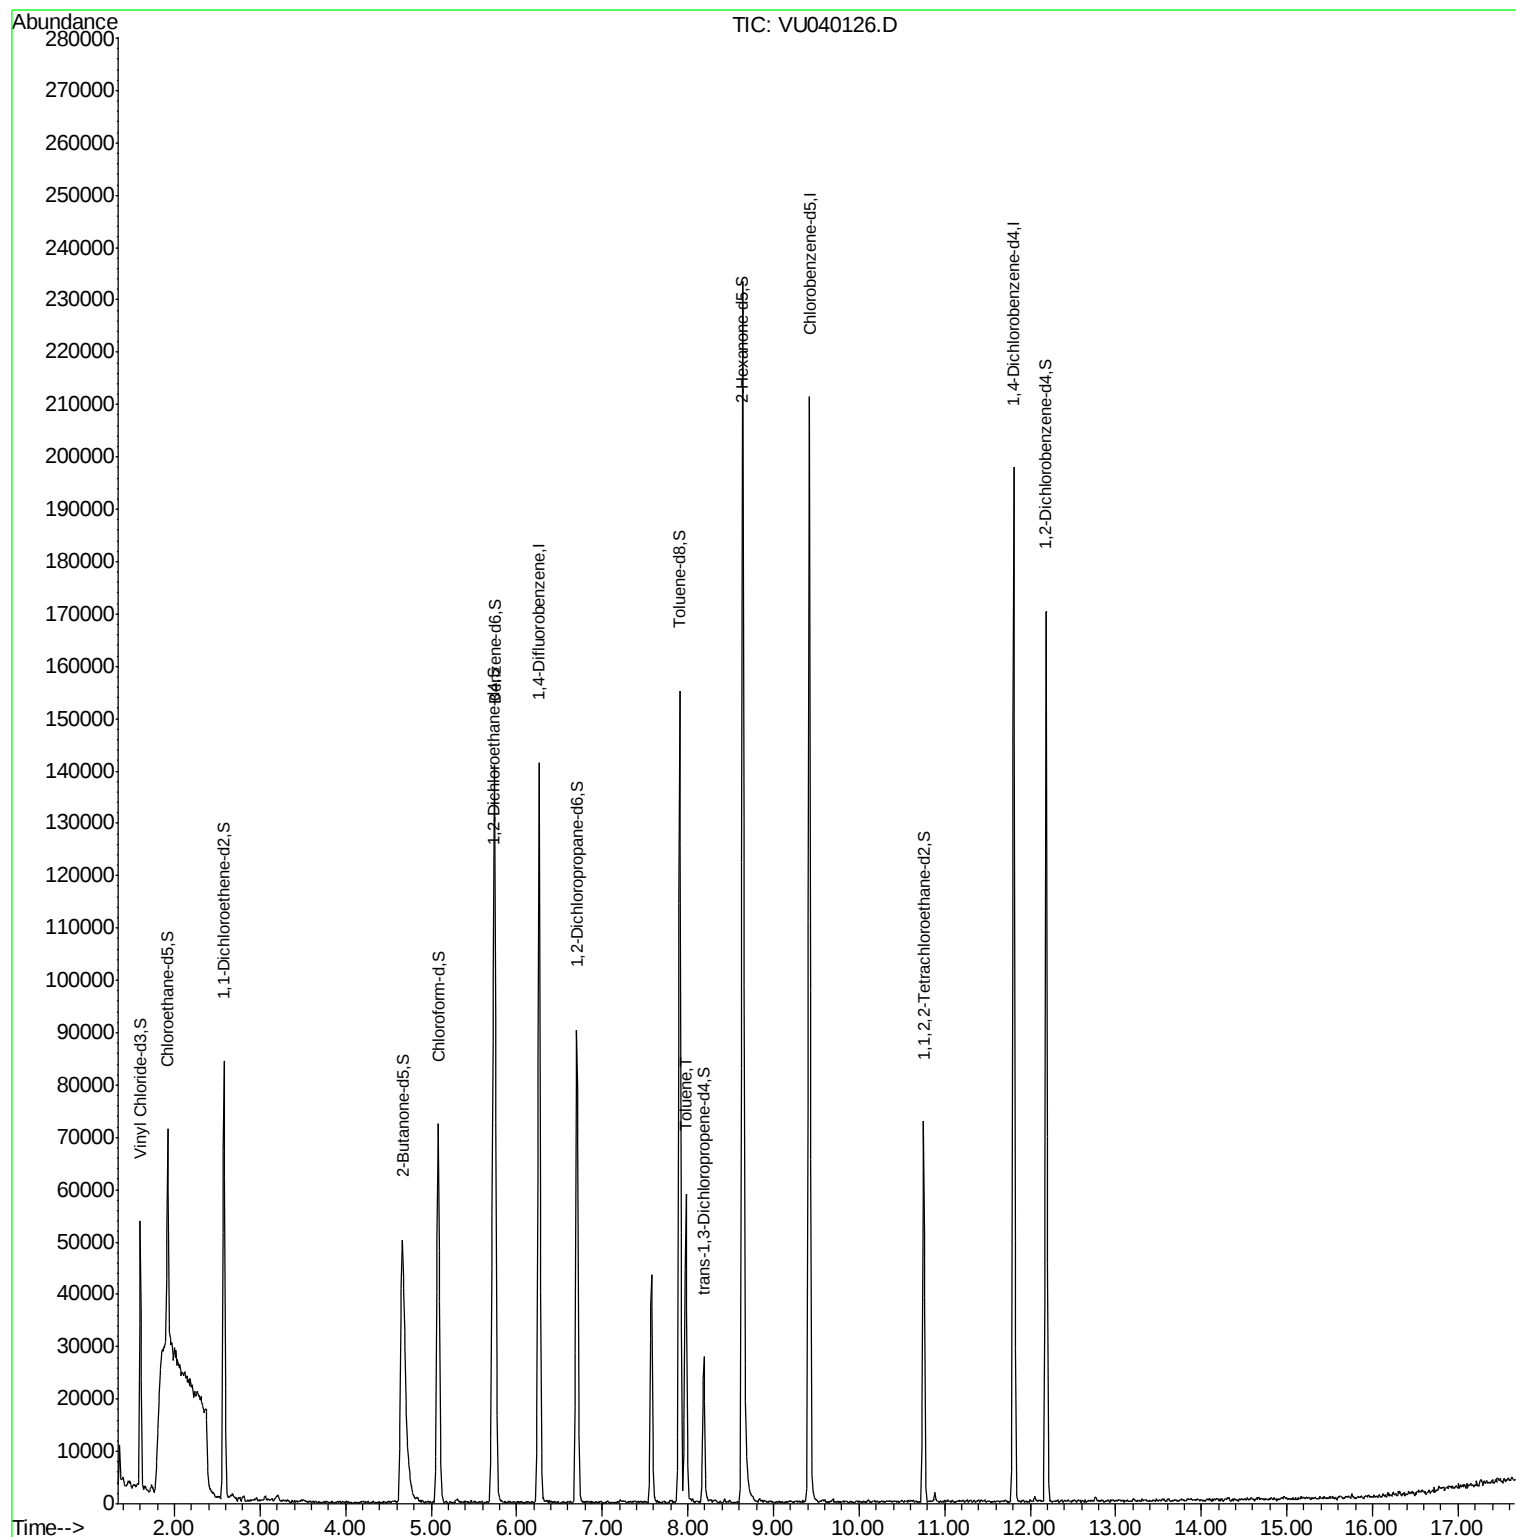

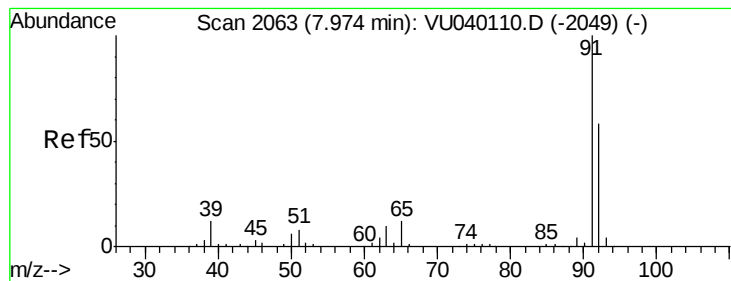

#42

Toluene

Concen: 1.013 ug/L

RT: 7.98 min Scan# 2064

Delta R.T. 0.00 min

Lab File: VU040126.D

Acq: 14 Sep 2020 18:21

Instrument :
MSVOA_U
ClientSampleId :
ETYP0

Tot Ion: 91 Resp: 39272

Ion Ratio Lower Upper

91 100

92 60.3 40.7 75.5

