

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU091420\
 Data File : VU040123.D
 Acq On : 14 Sep 2020 16:25
 Operator : SY/MD
 Sample : L3950-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFWT1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.527	51	58	69	rVB	28899	31446	7.64%	0.949%
2	1.604	74	82	94	rVB	43954	47515	11.55%	1.434%
3	1.922	172	181	195	rVB	36353	48768	11.85%	1.472%
4	2.465	342	350	361	rVB2	17386	28421	6.91%	0.858%
5	2.578	374	385	398	rBV	78907	127319	30.95%	3.842%
6	4.661	1016	1033	1059	rBV	41493	161565	39.27%	4.875%
7	4.825	1077	1084	1100	rVB3	6613	14728	3.58%	0.444%
8	5.083	1149	1164	1192	rVB3	68020	161237	39.19%	4.865%
9	5.742	1346	1369	1387	rBV4	130082	340947	82.87%	10.288%
10	6.176	1491	1504	1517	rBV3	3966	9147	2.22%	0.276%
11	6.263	1517	1531	1550	rVB	147807	273223	66.41%	8.245%
12	6.703	1654	1668	1687	rBV2	85121	165613	40.25%	4.997%
13	7.182	1798	1817	1828	rBV4	2867	5631	1.37%	0.170%
14	7.574	1925	1939	1954	rBV2	42784	73837	17.95%	2.228%
15	7.722	1973	1985	1999	rVB6	7112	13431	3.26%	0.405%
16	7.906	2029	2042	2056	rBV	144693	250574	60.91%	7.561%
17	8.185	2117	2129	2144	rBV2	26944	47281	11.49%	1.427%
18	8.642	2256	2271	2297	rBV	221718	411414	100.00%	12.415%
19	8.809	2310	2323	2324	rBV4	3536	5345	1.30%	0.161%
20	9.420	2497	2513	2534	rBV	213920	355266	86.35%	10.720%
21	10.754	2915	2928	2940	rBV	67622	107867	26.22%	3.255%
22	11.687	3209	3218	3228	rVB4	2806	4210	1.02%	0.127%
23	11.806	3244	3255	3269	rVB	208753	333998	81.18%	10.079%
24	12.053	3322	3332	3345	rBV3	18049	31666	7.70%	0.956%
25	12.188	3362	3374	3386	rBV	156804	248874	60.49%	7.510%
26	12.883	3582	3590	3597	rBV7	6943	9443	2.30%	0.285%
27	13.201	3682	3689	3696	rBV4	3792	5189	1.26%	0.157%


Sum of corrected areas: 3313955

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091420\
Data File : VU040123.D
Acq On : 14 Sep 2020 16:25
Operator : SY/MD
Sample : L3950-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFWT1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

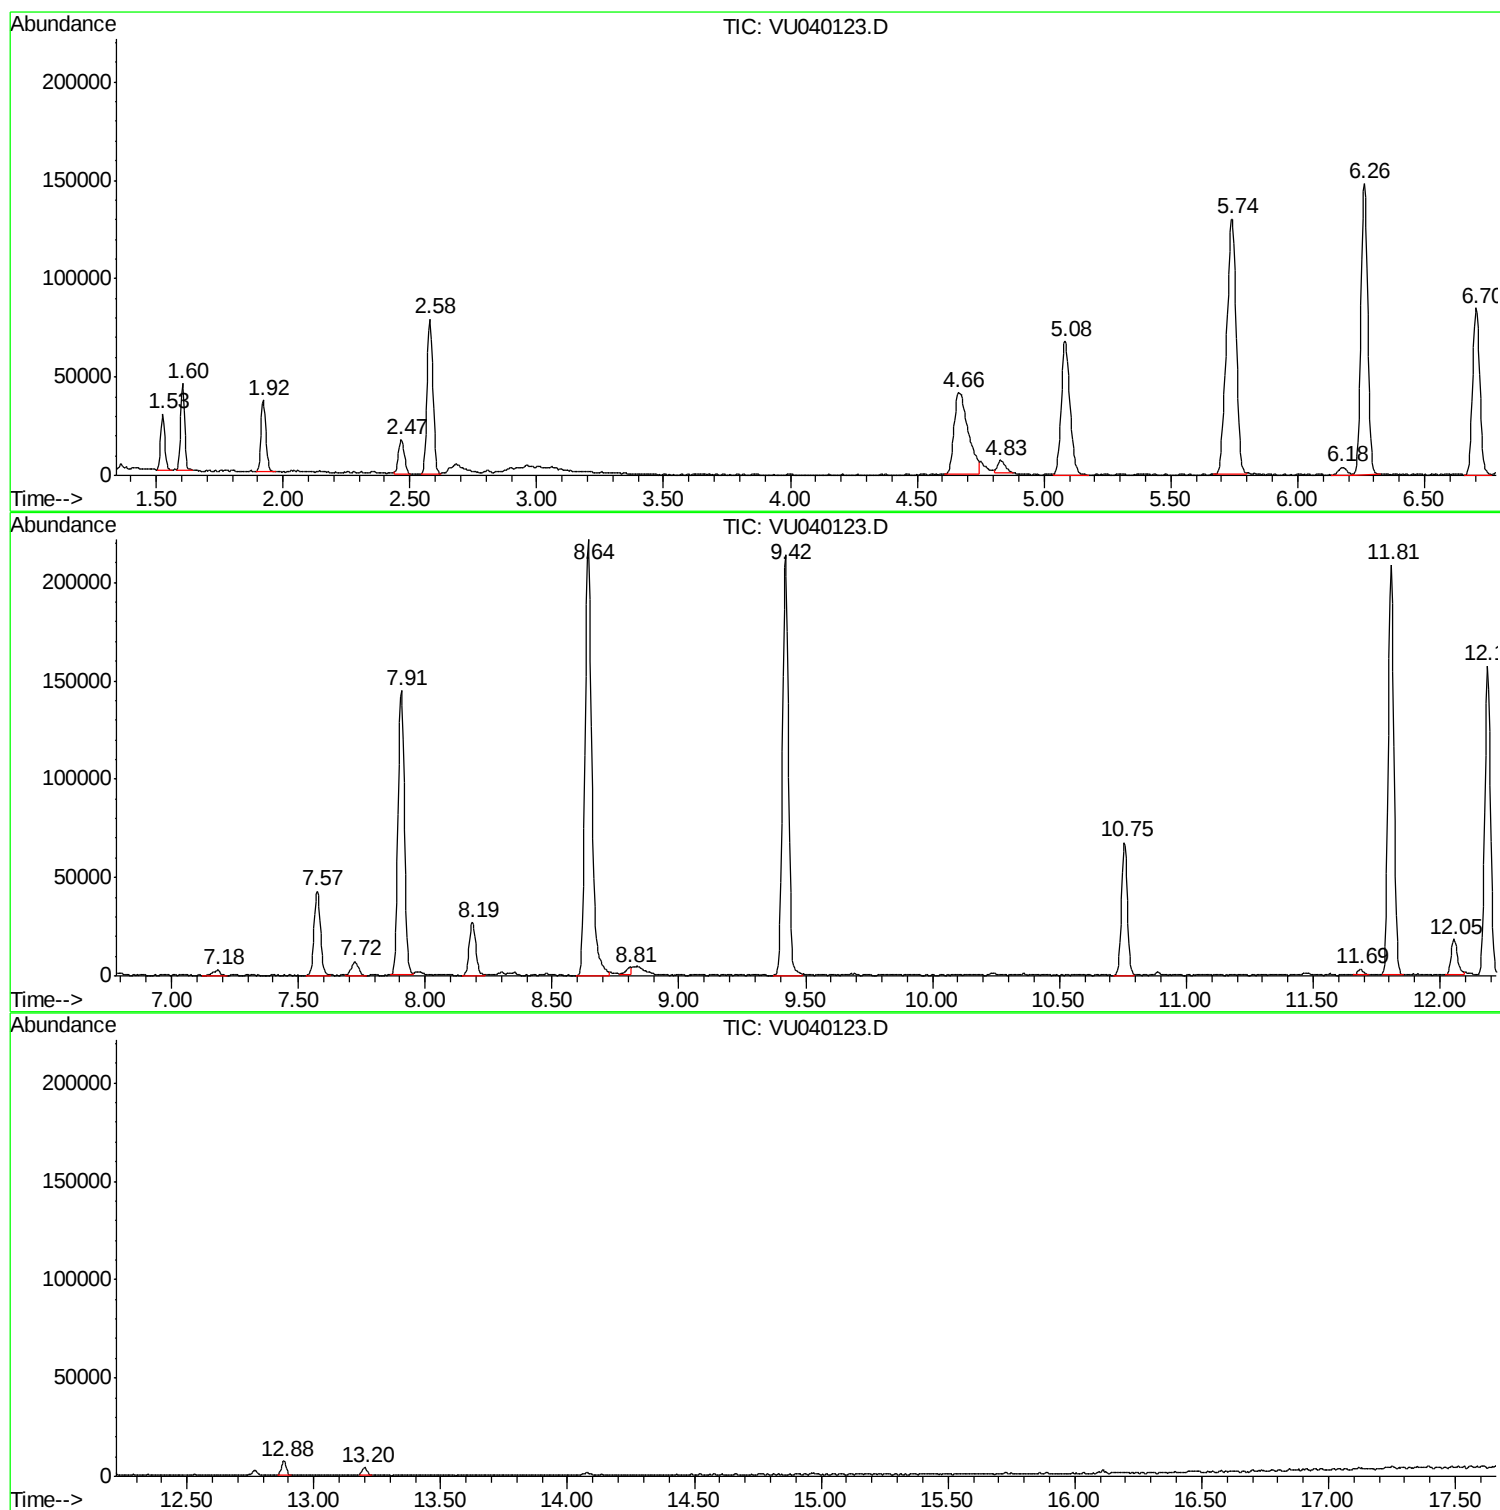

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091420\
Data File : VU040123.D
Acq On : 14 Sep 2020 16:25
Operator : SY/MD
Sample : L3950-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFWT1










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.47	0.52 ug/L	28421	1,4-Difluorobenzene	6.26

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Propane, 2-chloro-	78	C3H7Cl	000075-29-6	72
2		Propane, 2-chloro-	78	C3H7Cl	000075-29-6	58
3		2-Propyn-1-ol, acetate	98	C5H6O2	000627-09-8	9
4		Propane, 2-chloro-	78	C3H7Cl	000075-29-6	7
5		Propane, 2-nitro-	89	C3H7NO2	000079-46-9	4

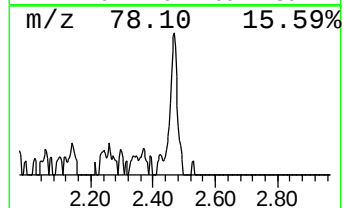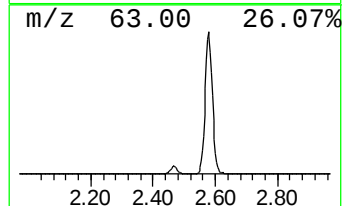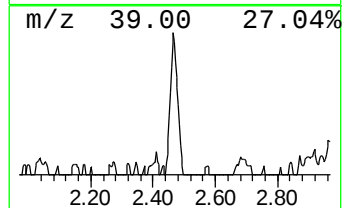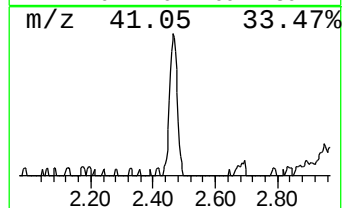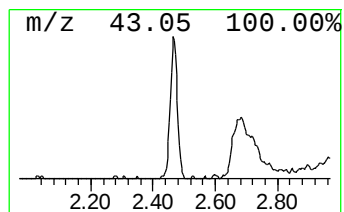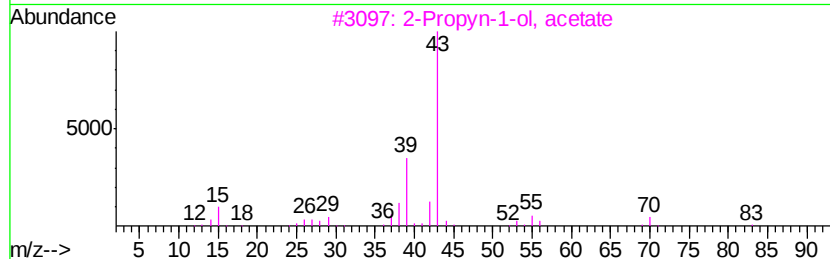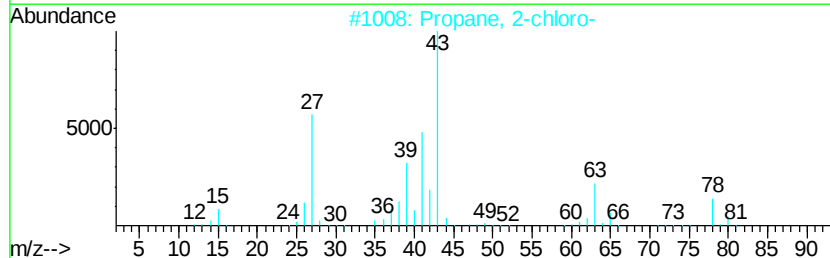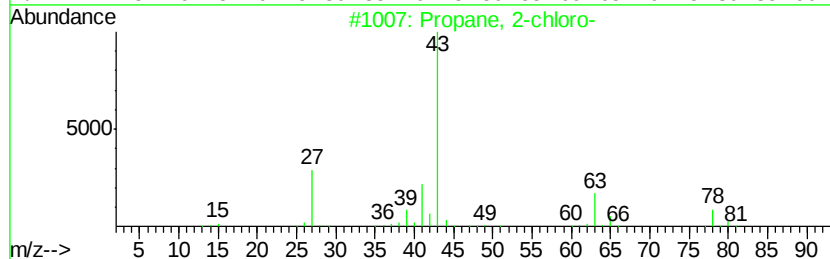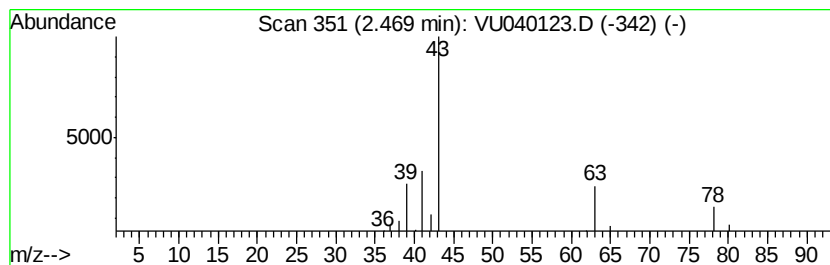

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU091420\
Data File : VU040123.D
Acq On : 14 Sep 2020 16:25
Operator : SY/MD
Sample : L3950-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFWT1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.47	0.5	ug/L	28421	1	6.26	273223	5.0