


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU091420\
Data File : VU040109.D
Acq On : 14 Sep 2020 09:35
Operator : SY/MD
Sample : BFB31
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB31

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Sep 15 04:05:49 2020

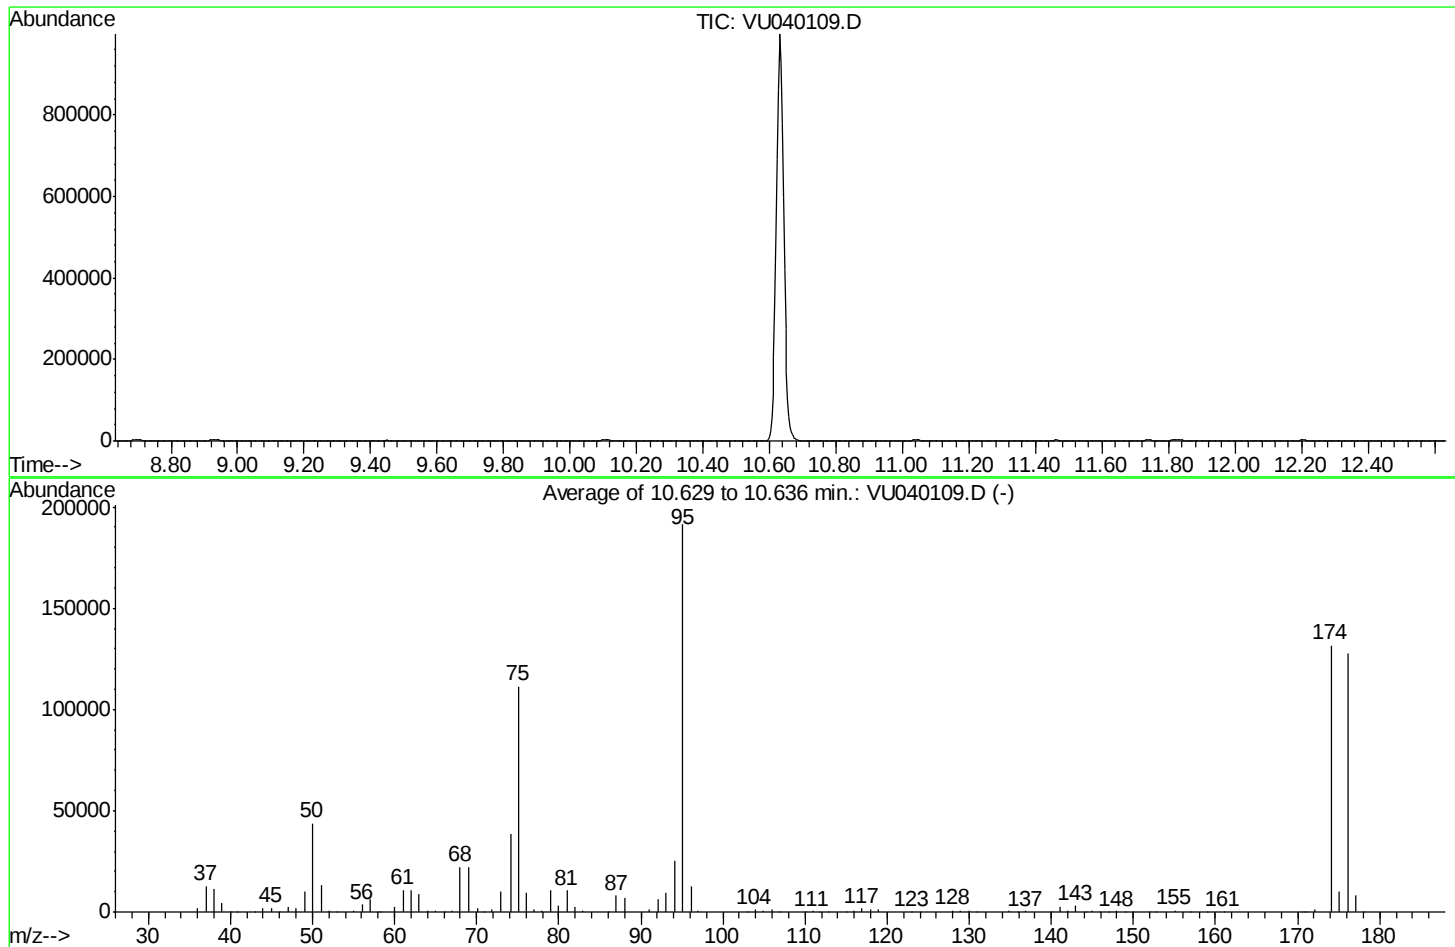

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	43685	PASS
75	95	30	80	58.2	111480	PASS
95	95	100	100	100.0	191466	PASS
96	95	5	9	6.5	12525	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.7	131602	PASS
175	174	5	9	7.7	10118	PASS
176	174	95	101	97.1	127850	PASS
177	176	5	9	6.3	8071	PASS

Scan 2875 (10.584 min): VU040109.D
BFB31

m/z	Abundance
44.00	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	2482.0
37.00	13310.0
38.00	11801.0
39.00	4568.0
40.00	325.0
43.10	128.0
44.00	2190.0
45.00	2290.0
46.00	314.0
47.00	2393.0
48.00	1695.0
49.00	10539.0
50.00	44904.0
51.10	13797.0
52.00	660.0
53.00	123.0
55.00	762.0
56.00	3824.0
57.10	6777.0
58.00	167.0
60.10	2473.0
61.00	11075.0
62.00	10985.0
63.00	8879.0
64.00	1096.0
65.00	903.0
66.00	156.0
67.10	835.0
68.00	22400.0
69.00	23080.0
70.10	1839.0
70.90	104.0
71.90	1695.0
73.00	10366.0
74.10	38696.0
75.10	113048.0
76.10	10380.0
77.10	965.0
78.00	770.0
79.00	10905.0
80.00	3072.0
81.00	10933.0
81.90	2635.0
82.90	365.0
87.00	8529.0
88.00	7213.0
91.00	1057.0
92.00	6575.0
93.10	10458.0
94.10	26056.0
95.10	193088.0
96.10	13120.0
97.00	445.0
104.00	1210.0
104.90	407.0
105.90	1276.0
106.90	277.0
110.10	152.0
110.90	423.0
111.80	171.0
112.80	307.0
115.00	286.0
115.90	977.0
117.00	1751.0
118.00	998.0
119.00	1382.0
123.00	140.0
124.10	197.0
128.00	918.0
129.00	381.0
130.00	733.0
131.00	308.0
134.80	393.0
137.00	511.0
139.90	242.0
141.00	2492.0
142.10	275.0
143.00	2914.0
144.20	135.0
145.00	481.0
145.90	317.0
147.00	118.0
148.00	496.0
149.00	132.0
149.90	186.0
155.10	503.0
157.00	273.0
158.90	149.0
161.00	247.0
170.90	222.0
172.20	1313.0
174.10	129432.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

175.10	10138.0
176.10	125024.0
177.10	8340.0
178.00	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	2244.0
37.00	13074.0
38.00	12005.0
39.00	4699.0
40.00	274.0
40.80	104.0
43.00	166.0
44.00	2068.0
45.00	2223.0
46.00	313.0
47.00	2454.0
48.00	1844.0
49.00	10429.0
50.00	45232.0
51.10	14043.0
52.10	665.0
55.00	750.0
56.10	3888.0
57.10	6834.0
58.20	239.0
60.00	2387.0
61.00	11503.0
62.00	10828.0
63.00	8976.0
64.00	928.0
65.00	693.0
66.10	142.0
67.00	737.0
68.00	22888.0
69.00	22896.0
70.00	1927.0
70.90	179.0
71.90	1737.0
73.00	10810.0
74.10	39648.0
75.10	115008.0
76.10	10108.0
77.10	1086.0
78.00	740.0
79.00	10956.0
80.00	3118.0
81.00	11114.0
81.90	2697.0
83.00	368.0
86.10	329.0
87.00	8570.0
88.00	7361.0
90.90	1051.0
92.10	6799.0
93.00	9976.0
94.10	26544.0
95.10	197376.0
96.10	12943.0
97.00	462.0
103.00	117.0
103.90	1243.0
104.90	423.0
105.90	1248.0
107.00	273.0
110.00	176.0
110.90	428.0
111.80	137.0
112.90	279.0
115.00	269.0
115.90	892.0
117.00	1866.0
118.00	1021.0
119.00	1387.0
124.00	234.0
128.00	982.0
129.00	424.0
130.00	678.0
131.00	305.0
134.80	419.0
135.80	106.0
136.90	482.0
139.90	194.0
141.00	2733.0
142.10	365.0
143.00	3199.0
144.20	190.0
145.00	572.0
145.80	334.0
147.00	114.0
148.00	536.0
149.00	188.0
149.90	150.0
151.90	103.0
152.80	121.0
155.00	661.0
157.00	342.0
159.00	185.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

160.90	248.0
171.10	187.0
172.10	1159.0
174.10	136320.0
175.10	10472.0
176.10	132032.0
177.10	8340.0
178.00	236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	1943.0
37.00	11727.0
38.00	10737.0
39.00	4403.0
40.00	200.0
43.00	160.0
44.00	1810.0
45.00	1940.0
46.00	251.0
47.00	2185.0
48.00	1674.0
49.00	9345.0
50.00	40920.0
51.10	12804.0
52.10	656.0
55.00	737.0
56.10	3532.0
57.10	6211.0
58.20	301.0
60.00	2224.0
61.00	10666.0
62.00	10090.0
63.00	8384.0
64.10	835.0
65.00	590.0
66.10	147.0
66.90	590.0
68.00	21168.0
69.00	20352.0
70.00	1847.0
70.90	196.0
71.90	1309.0
73.00	9793.0
74.10	36808.0
75.10	106384.0
76.10	8668.0
77.00	1004.0
77.90	622.0
79.00	9975.0
80.00	2761.0
81.00	10097.0
82.00	2550.0
83.00	332.0
86.00	340.0
87.00	7497.0
88.00	6714.0
90.90	964.0
92.10	6334.0
93.10	8584.0
94.10	24128.0
95.10	183936.0
96.10	11512.0
97.00	367.0
102.90	139.0
103.90	1225.0
104.90	360.0
106.00	1141.0
107.00	220.0
109.90	223.0
110.90	392.0
112.90	292.0
115.00	190.0
116.00	771.0
116.90	1850.0
117.90	971.0
119.00	1245.0
124.00	219.0
128.00	929.0
128.90	409.0
129.90	617.0
130.90	314.0
134.90	347.0
135.90	132.0
136.80	460.0
139.90	142.0
141.00	2766.0
142.00	442.0
143.00	2998.0
144.20	208.0
145.00	551.0
145.80	316.0
147.90	520.0
149.10	178.0
149.90	140.0
152.80	143.0
155.00	765.0
157.00	346.0
159.00	203.0
160.90	201.0
170.60	155.0
172.10	918.0
174.10	129056.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

175.10	9745.0
176.10	126496.0
177.10	7533.0
178.00	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31