

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU091421\  
 Data File : VU044630.D  
 Acq On : 14 Sep 2021 16:57  
 Operator : SY/MD  
 Sample : M3739-04  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 C0B77

Quant Time: Sep 15 01:44:33 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR090921WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Sep 15 01:41:41 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.256  | 114   | 149395   | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 9.423  | 117   | 154772   | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.816 | 152   | 74005    | 5.000    | ug/L   | 0.00     |
|                               |        |       |          |          |        |          |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.601  | 65    | 34989    | 3.969    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 79.400%  |
| 7) Chloroethane-d5            | 1.919  | 69    | 38300    | 4.258    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 85.200%  |
| 11) 1,1-Dichloroethene-d2     | 2.575  | 65    | 17492    | 3.929    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 78.600%  |
| 20) 2-Butanone-d5             | 4.642  | 46    | 162996   | 44.111   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 88.220%  |
| 24) Chloroform-d              | 5.070  | 84    | 80125    | 4.321    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 86.400%  |
| 26) 1,2-Dichloroethane-d4     | 5.710  | 65    | 48608    | 4.397    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 88.000%  |
| 32) Benzene-d6                | 5.735  | 84    | 159958   | 4.053    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 81.000%  |
| 36) 1,2-Dichloropropane-d6    | 6.697  | 67    | 54338    | 4.193    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 83.800%  |
| 41) Toluene-d8                | 7.902  | 98    | 127927   | 3.724    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 74.400%  |
| 43) trans-1,3-Dichloroprop... | 8.185  | 79    | 17243    | 3.774    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 75.400%  |
| 46) 2-Hexanone-d5             | 8.642  | 63    | 124457   | 42.387   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 84.780%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.761 | 84    | 46693    | 4.063    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 81.200%  |
| 66) 1,2-Dichlorobenzene-d4    | 12.198 | 152   | 49218    | 4.030    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 80.600%  |
|                               |        |       |          |          |        |          |
| Target Compounds              |        |       |          |          | Qvalue |          |
| 13) Acetone                   | 2.649  | 43    | 7438     | 3.091    | ug/L   | 89       |
| -----                         |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU091421\  
Data File : VU044630.D  
Acq On : 14 Sep 2021 16:57  
Operator : SY/MD  
Sample : M3739-04  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
C0B77

Quant Time: Sep 15 01:44:33 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR090921WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Wed Sep 15 01:41:41 2021  
Response via : Initial Calibration

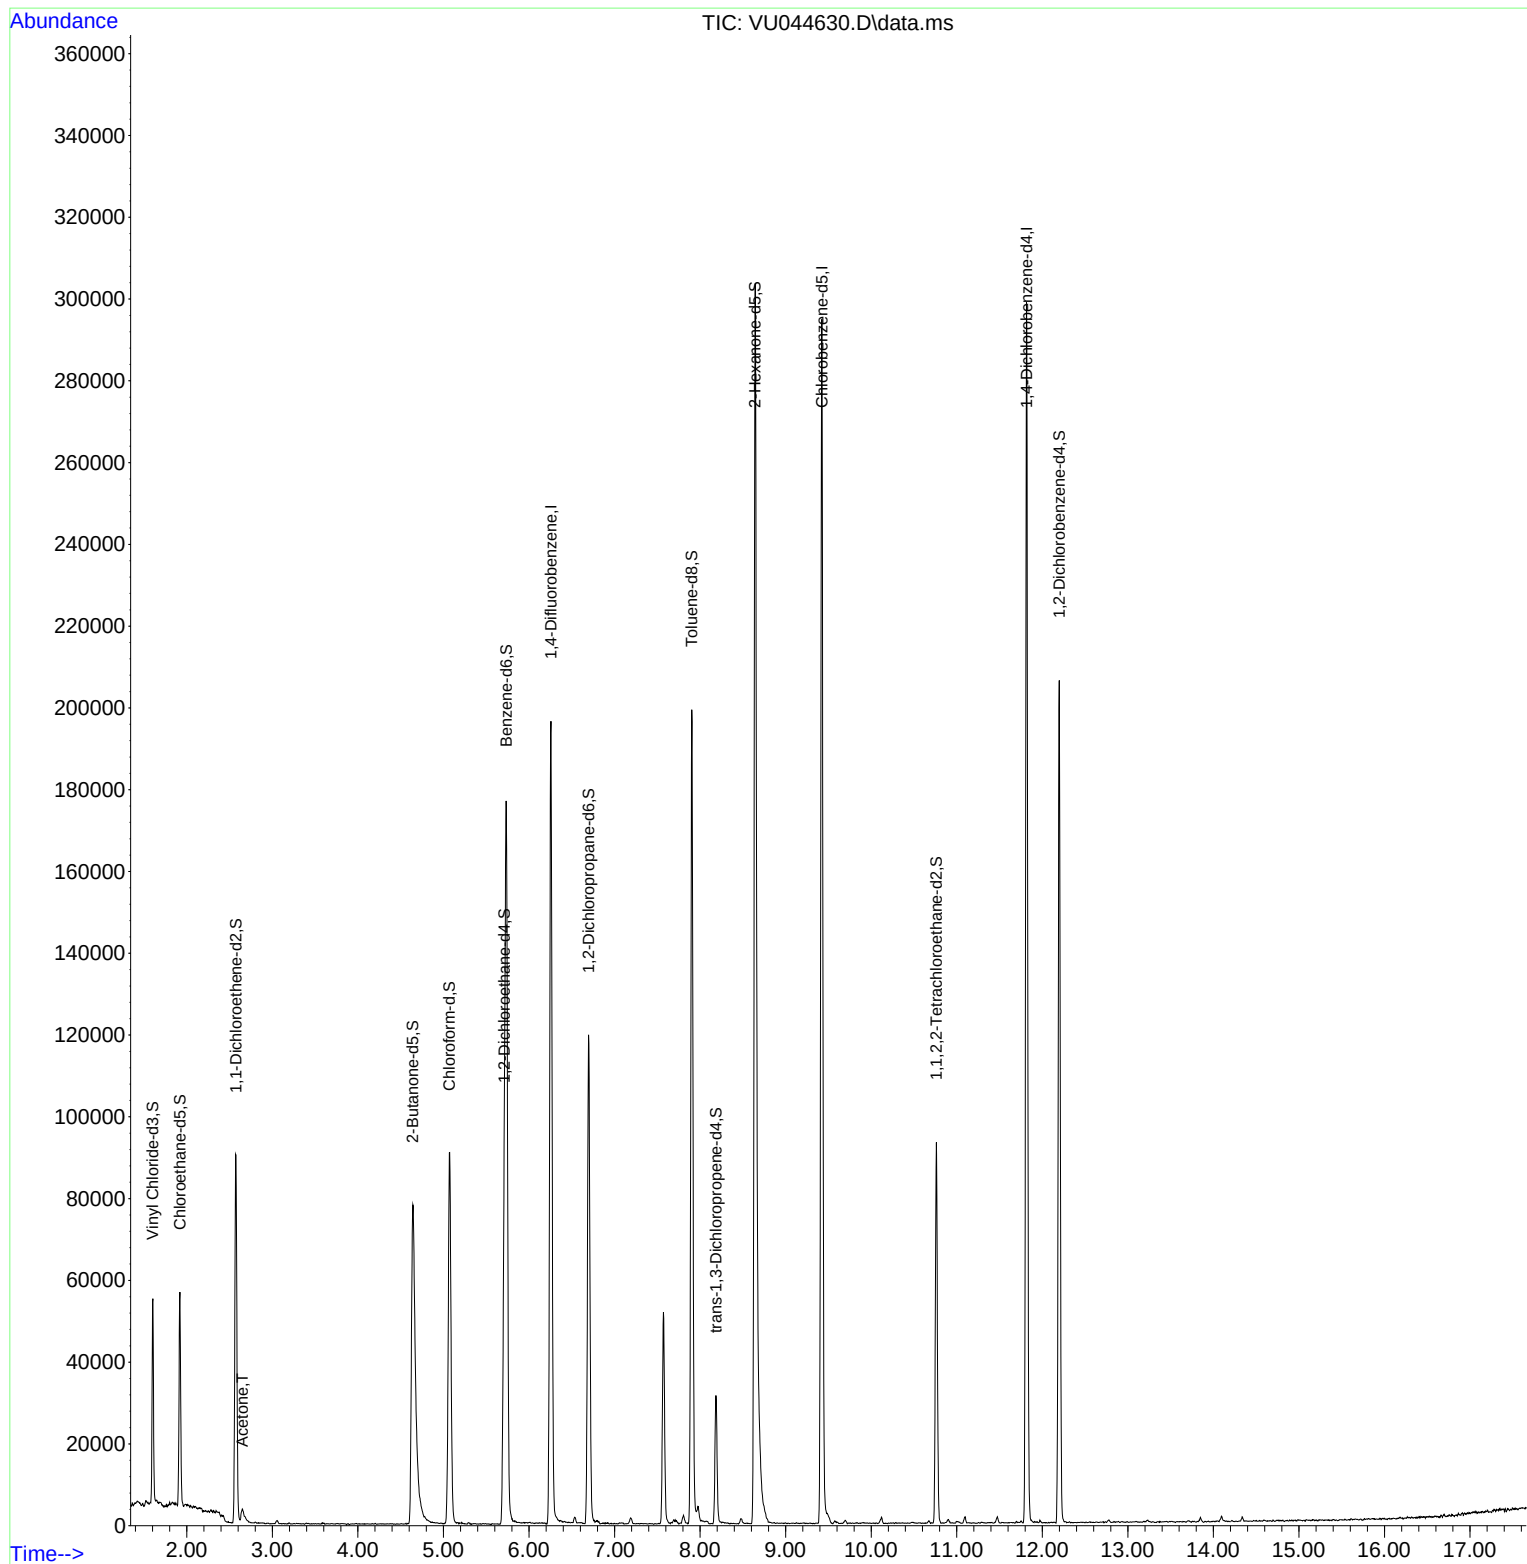

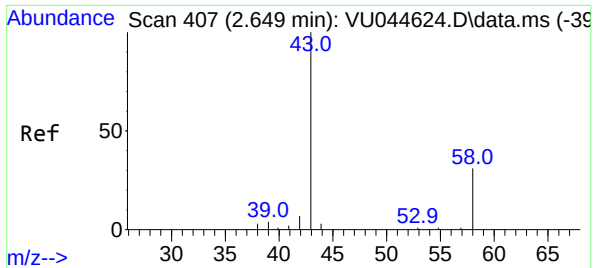

#13  
 Acetone  
 Concen: 3.091 ug/L  
 RT: 2.649 min Scan# 407  
 Delta R.T. 0.000 min  
 Lab File: VU044630.D  
 Acq: 14 Sep 2021 16:57

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 C0B77

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 7438  |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 58       | 26.3  | 0.0   | 42.4  |

