

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091421\
 Data File : VU044632.D
 Acq On : 14 Sep 2021 17:45
 Operator : SY/MD
 Sample : M3739-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B68

Quant Time: Sep 15 01:44:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 15 01:41:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	132855	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	136201	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	62106	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	33887	4.323	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	86.400%	
7) Chloroethane-d5	1.919	69	37497	4.687	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.800%	
11) 1,1-Dichloroethene-d2	2.571	65	17365	4.386	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	87.800%	
20) 2-Butanone-d5	4.645	46	160817	48.939	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	97.880%	
24) Chloroform-d	5.070	84	78963	4.789	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.800%	
26) 1,2-Dichloroethane-d4	5.710	65	48563	4.939	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.800%	
32) Benzene-d6	5.735	84	157087	4.523	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	6.700	67	54712	4.797	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.000%	
41) Toluene-d8	7.902	98	128369	4.246	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.000%	
43) trans-1,3-Dichloroprop...	8.185	79	16859	4.193	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.800%	
46) 2-Hexanone-d5	8.645	63	122032	47.228	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.460%	
56) 1,1,2,2-Tetrachloroeth...	10.761	84	46777	4.626	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.600%	
66) 1,2-Dichlorobenzene-d4	12.198	152	49275	4.808	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.200%	
Target Compounds					Qvalue	
25) Chloroform	5.096	83	5685	0.291	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091421\
Data File : VU044632.D
Acq On : 14 Sep 2021 17:45
Operator : SY/MD
Sample : M3739-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B68

Quant Time: Sep 15 01:44:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 15 01:41:41 2021
Response via : Initial Calibration

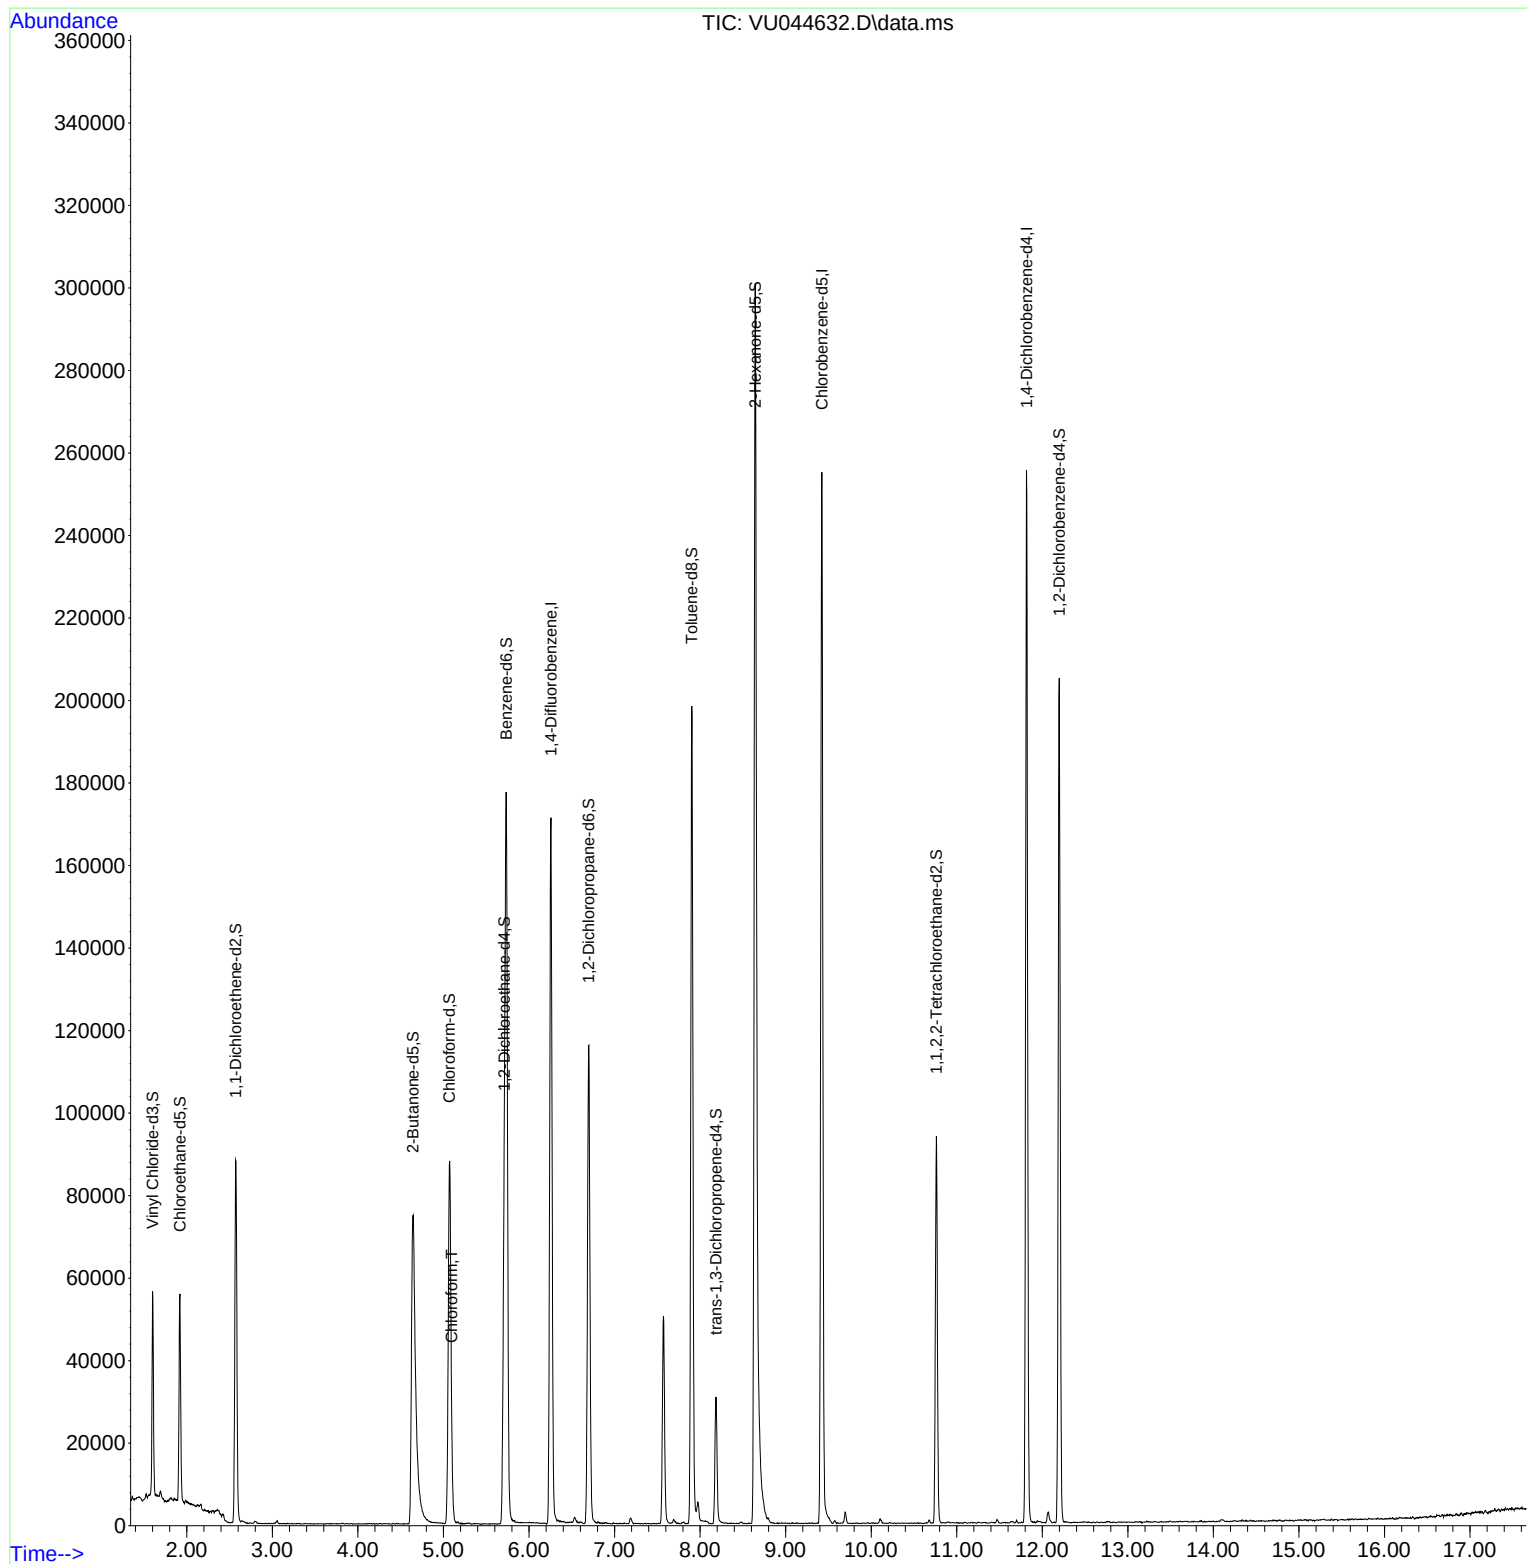

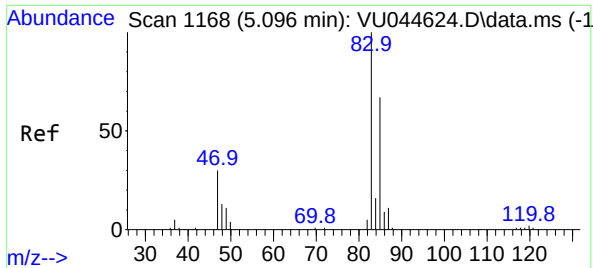

#25
Chloroform
Concen: 0.291 ug/L
RT: 5.096 min Scan# 1168
Delta R.T. -0.000 min
Lab File: VU044632.D
Acq: 14 Sep 2021 17:45

Instrument :
MSVOA_U
ClientSampleId :
C0B68

Tgt Ion: 83 Resp: 5685
Ion Ratio Lower Upper
83 100
85 61.7 44.2 82.0

