


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091421\
 Data File : VU044623.D
 Acq On : 14 Sep 2021 10:33
 Operator : SY/MD
 Sample : BFB017
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB017

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Sep 15 01:41:41 2021

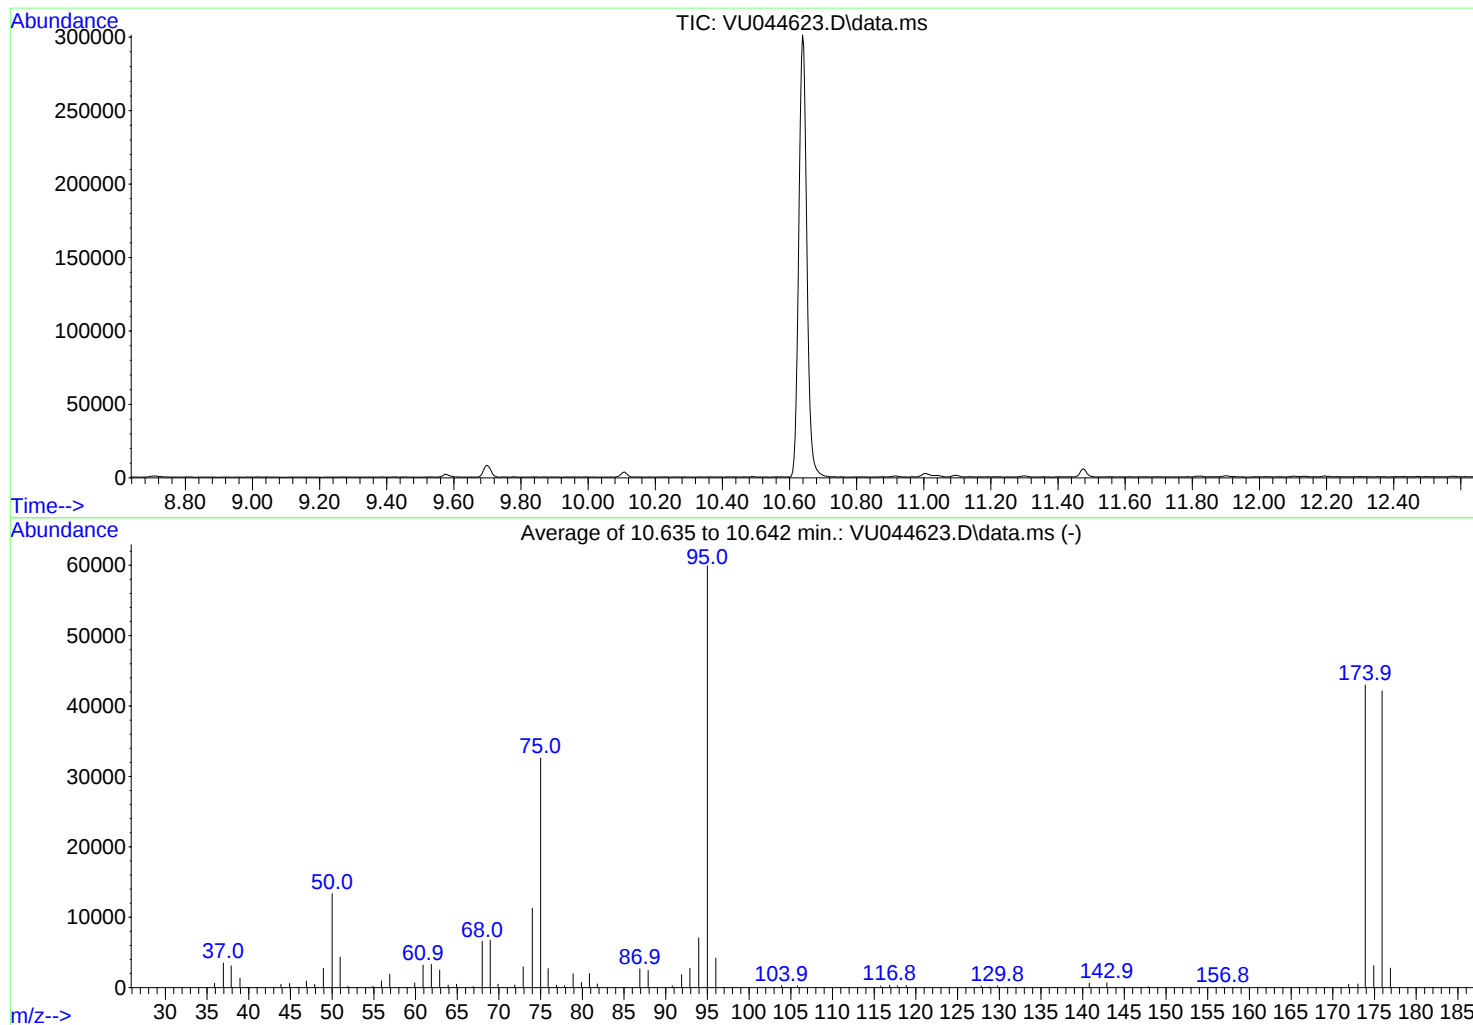

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	13335	PASS
75	95	30	80	54.4	32595	PASS
95	95	100	100	100.0	59925	PASS
96	95	5	9	7.0	4174	PASS
173	174	0.00	2	1.2	522	PASS
174	95	50	120	71.8	42997	PASS
175	174	5	9	7.3	3144	PASS
176	174	95	101	98.1	42173	PASS
177	176	5	9	6.6	2781	PASS

m/z	Abundance
35.90	576.0
36.90	3390.0
37.90	3143.0
39.00	1358.0
39.80	179.0
43.90	882.0
44.90	570.0
46.90	872.0
47.90	424.0
48.90	2698.0
50.00	13211.0
50.90	4322.0
51.90	222.0
54.90	221.0
55.90	1008.0
56.90	1937.0
59.90	661.0
60.90	3005.0
61.90	3355.0
62.90	2480.0
63.90	378.0
64.90	475.0
66.90	185.0
68.00	6544.0
68.90	6596.0
69.90	497.0
71.90	372.0
72.90	2945.0
74.00	11197.0
75.00	32272.0
75.90	2728.0
76.90	396.0
77.80	290.0
78.90	1936.0
79.90	754.0
80.90	1968.0
81.80	504.0
86.90	2699.0
87.90	2500.0
90.80	246.0
91.90	1765.0
92.90	2791.0
93.90	6999.0
95.00	60040.0
96.00	4202.0
96.90	138.0
103.90	296.0
105.80	297.0
115.80	253.0
116.80	347.0
117.80	225.0
118.80	330.0
127.80	252.0
128.80	103.0
129.80	270.0
130.80	111.0
140.80	581.0
142.90	669.0
147.80	150.0
171.90	473.0
173.00	543.0
173.90	43896.0
174.90	3279.0
175.90	43336.0
176.90	2764.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

Scan 2878 (10.594 min): VU044623.D\data.ms
BFB017

m/z	Abundance
39.90	188.0
43.80	421.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
35.90	648.0
37.00	3526.0
37.90	2961.0
38.90	1235.0
39.90	215.0
43.90	902.0
44.90	583.0
45.80	102.0
46.90	913.0
47.90	446.0
49.00	2703.0
50.00	13081.0
51.00	4231.0
51.90	185.0
54.90	180.0
55.90	903.0
56.90	1832.0
59.90	714.0
60.90	3284.0
61.90	3096.0
62.90	2476.0
63.90	322.0
64.90	484.0
66.90	131.0
68.00	6366.0
69.00	6690.0
69.90	457.0
71.90	374.0
72.90	2839.0
74.00	11103.0
75.00	32000.0
75.90	2625.0
76.90	342.0
77.90	252.0
78.90	1904.0
79.90	695.0
80.80	2016.0
81.80	515.0
86.90	2546.0
87.90	2340.0
90.80	237.0
91.90	1842.0
92.90	2573.0
94.00	7018.0
95.00	58056.0
96.00	4003.0
103.90	274.0
105.80	250.0
115.80	192.0
116.90	357.0
117.80	261.0
118.90	300.0
127.90	195.0
128.80	118.0
129.80	211.0
136.70	109.0
140.80	654.0
142.90	673.0
144.80	119.0
147.90	113.0
156.80	112.0
171.90	410.0
173.00	489.0
173.90	40968.0
174.90	2956.0
175.90	39656.0
176.90	2725.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
35.90	644.0
36.90	3621.0
37.90	3193.0
39.00	1333.0
39.80	190.0
43.90	924.0
44.90	611.0
45.80	100.0
46.90	972.0
47.90	464.0
49.00	2804.0
50.00	13713.0
50.90	4415.0
51.90	218.0
54.90	209.0
55.90	988.0
56.90	1941.0
59.90	693.0
60.90	3311.0
61.90	3411.0
62.90	2565.0
63.90	373.0
64.90	488.0
66.90	172.0
68.00	6789.0
68.90	6970.0
69.90	525.0
71.90	393.0
72.90	2987.0
74.00	11581.0
75.00	33512.0
75.90	2775.0
76.90	386.0
77.80	286.0
78.90	2009.0
79.90	767.0
80.90	2046.0
81.80	534.0
86.90	2770.0
87.90	2462.0
90.80	244.0
91.90	1923.0
92.90	2856.0
93.90	7209.0
95.00	61680.0
96.00	4317.0
96.90	101.0
103.90	304.0
105.80	288.0
115.80	241.0
116.90	382.0
117.80	266.0
118.80	323.0
127.80	229.0
128.80	112.0
129.80	268.0
130.80	110.0
140.80	656.0
142.90	717.0
144.80	102.0
147.80	136.0
156.80	120.0
171.90	452.0
173.00	533.0
173.90	44128.0
174.90	3196.0
175.90	43528.0
176.90	2854.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017