

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
 Data File : VU055315.D
 Acq On : 14 Sep 2023 18:53
 Operator : MD/SY
 Sample : 04380-02 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4L3

Quant Time: Sep 15 03:04:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 15 02:53:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.248	114	173848	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	179963	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	85130	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	46448	5.701	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	114.000%	
7) Chloroethane-d5	1.908	69	46948	4.978	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.600%	
11) 1,1-Dichloroethene-d2	2.560	65	16928	3.646	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	73.000%	
20) 2-Butanone-d5	4.634	46	101121	42.767	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	85.540%	
24) Chloroform-d	5.062	84	86515	4.001	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.000%	
26) 1,2-Dichloroethane-d4	5.702	65	47897	4.428	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.600%	
32) Benzene-d6	5.724	84	171458	3.860	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	77.200%	
36) 1,2-Dichloropropane-d6	6.689	67	54701	3.872	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	77.400%	
41) Toluene-d8	7.898	98	144536	3.532	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	70.600%	
43) trans-1,3-Dichloroprop...	8.181	79	17840	4.585	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	91.800%	
46) 2-Hexanone-d5	8.631	63	56596	35.828	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	71.660%	
56) 1,1,2,2-Tetrachloroeth...	10.756	84	40179	4.044	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	80.800%	
66) 1,2-Dichlorobenzene-d4	12.193	152	49464	3.981	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	79.600%#	
Target Compounds						Qvalue
16) Methylene chloride	3.043	84	9269	0.755	ug/L	93
22) cis-1,2-Dichloroethene	4.666	96	2529	0.253	ug/L	87
34) Trichloroethene	6.541	95	5784	0.543	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
Data File : VU055315.D
Acq On : 14 Sep 2023 18:53
Operator : MD/SY
Sample : 04380-02 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4L3

Quant Time: Sep 15 03:04:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 15 02:53:52 2023
Response via : Initial Calibration




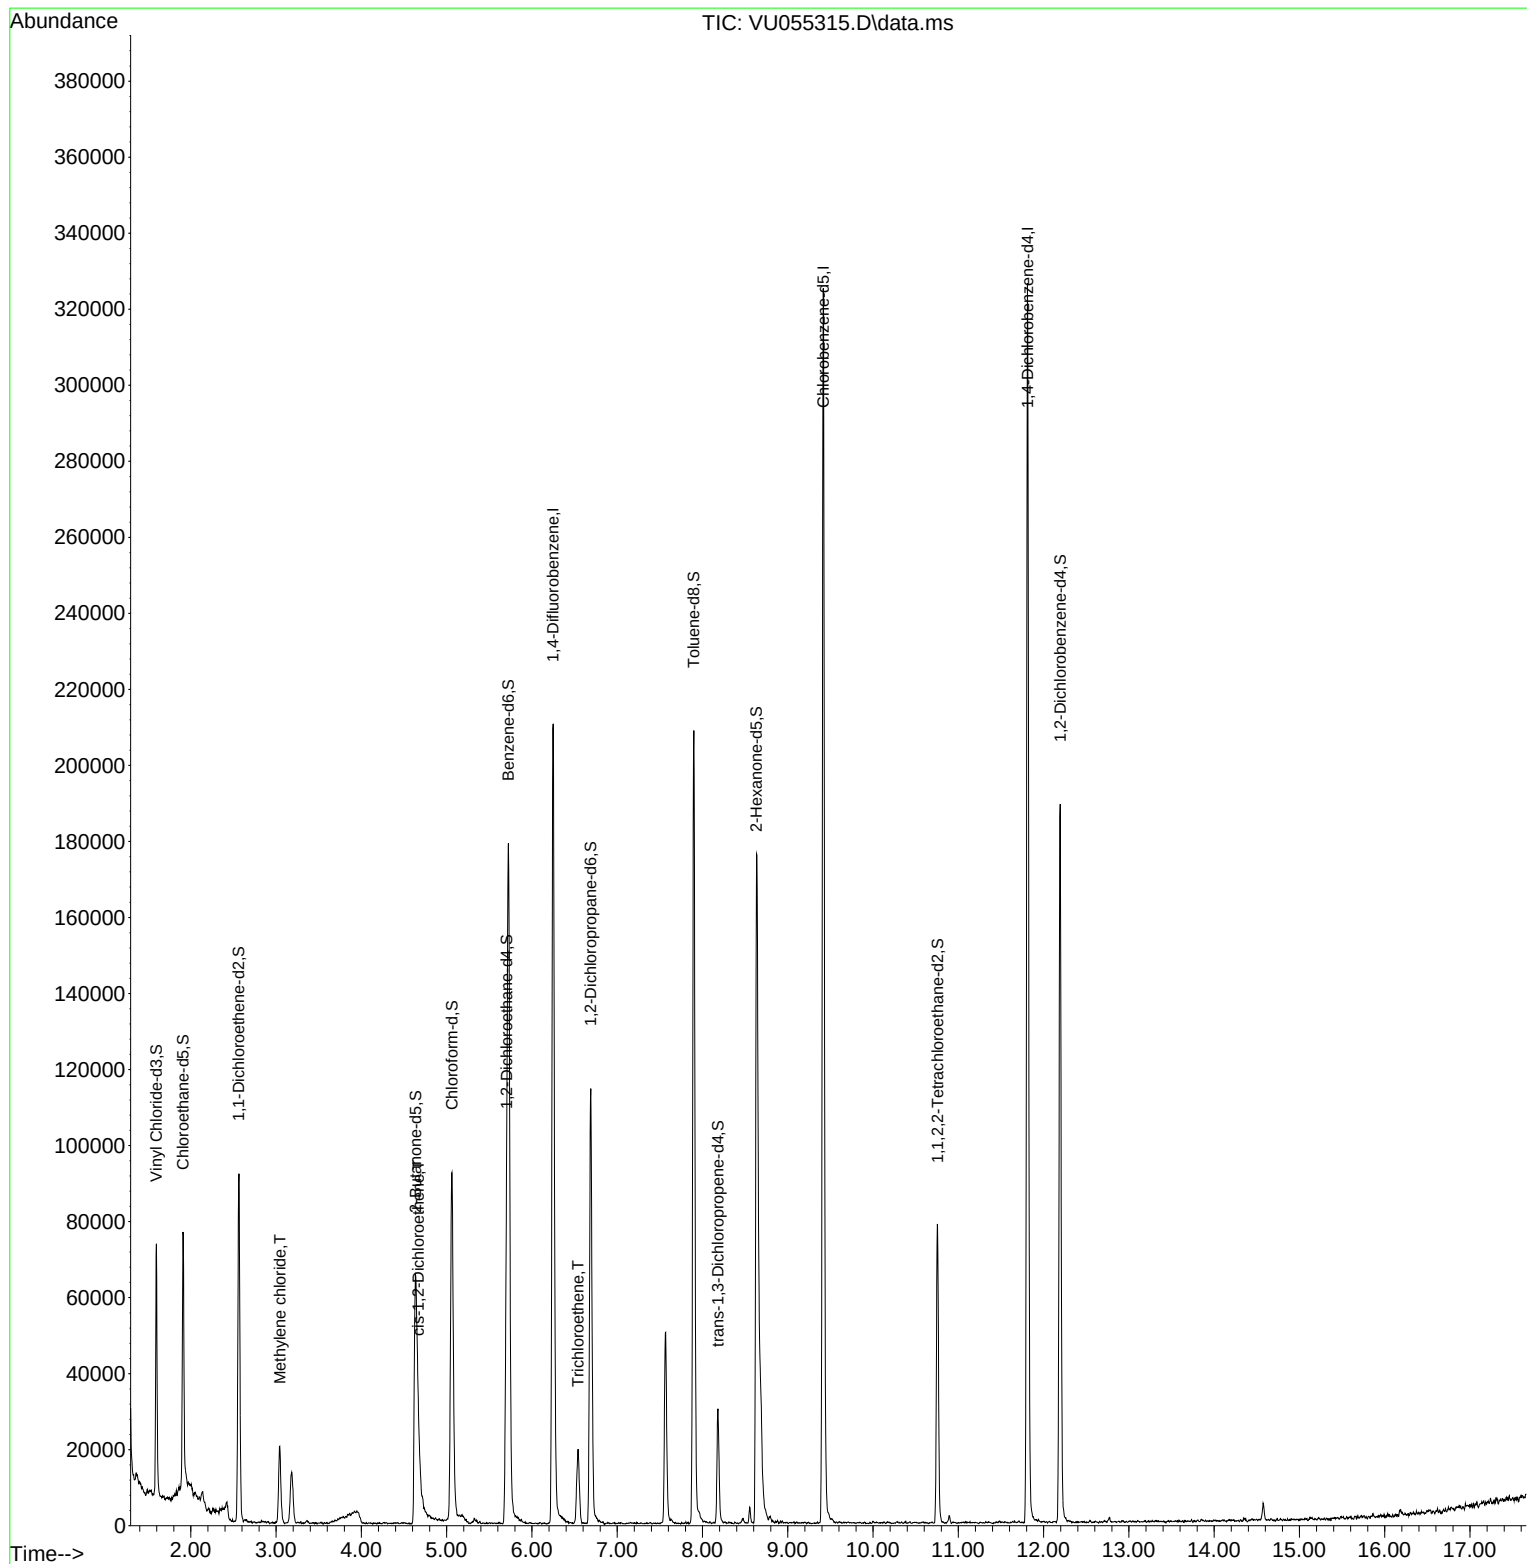


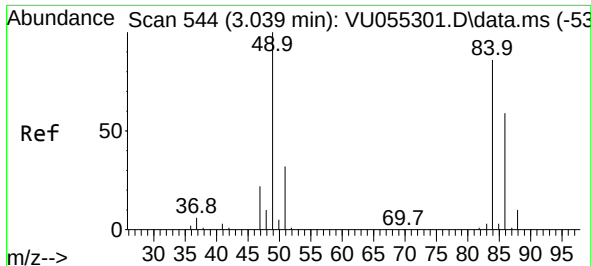

#16
Methylene chloride
Concen: 0.755 ug/L
RT: 3.043 min Scan# 54
Delta R.T. 0.003 min
Lab File: VU055315.D
Acq: 14 Sep 2023 18:53




Instrument :
MSVOA_U
ClientSampleId :
BH4L3


Tgt Ion: 84	Resp:	9269	
Ion	Ratio	Lower	Upper
84	100		
86	64.2	43.4	80.6
49	135.6	87.7	162.9

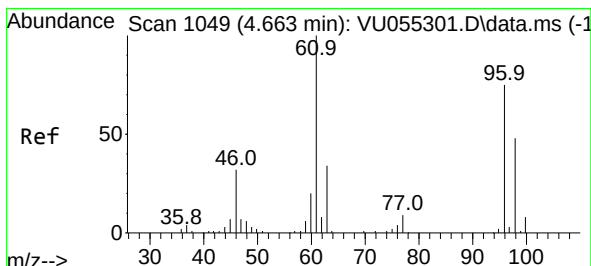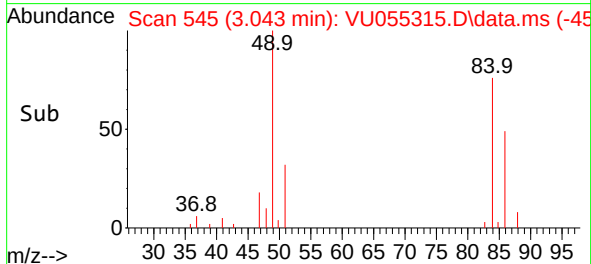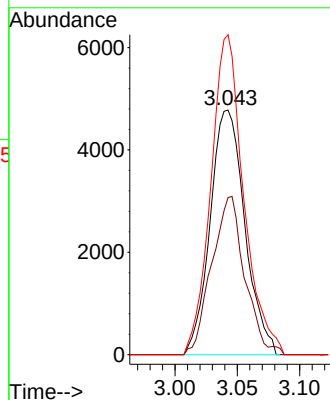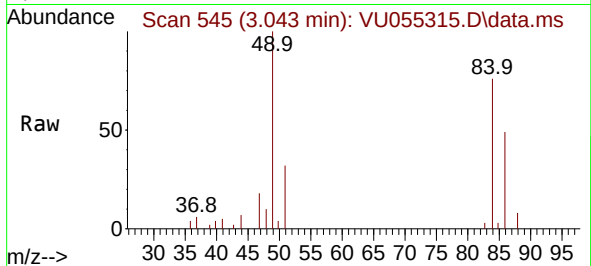

#22
cis-1,2-Dichloroethene
Concen: 0.253 ug/L
RT: 4.666 min Scan# 1050
Delta R.T. 0.003 min
Lab File: VU055315.D
Acq: 14 Sep 2023 18:53

Tgt Ion: 96	Resp:	2529	
Ion	Ratio	Lower	Upper
96	100		
61	118.9	97.2	180.4
98	60.7	46.1	85.7

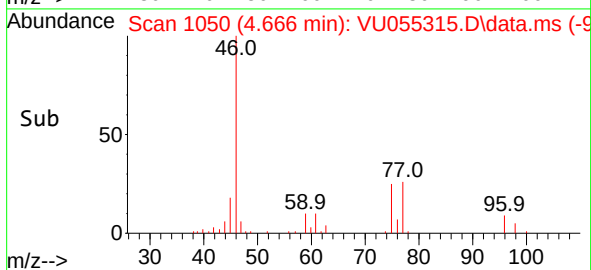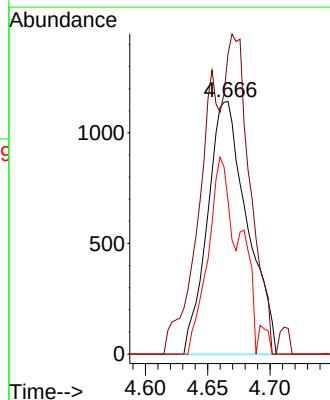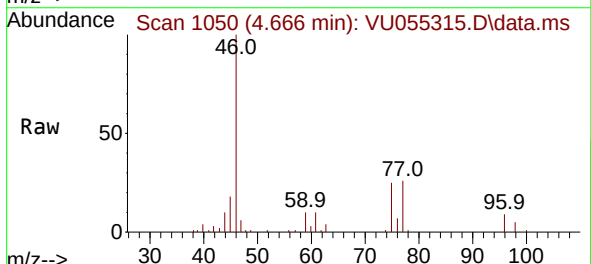

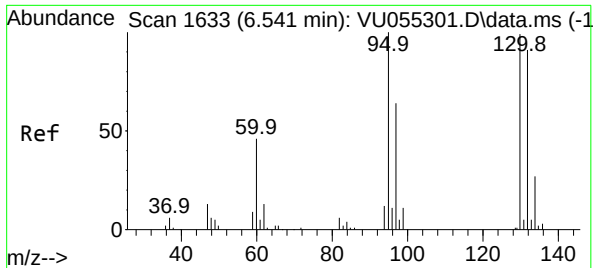

#34
 Trichloroethene
 Concen: 0.543 ug/L
 RT: 6.541 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU055315.D
 Acq: 14 Sep 2023 18:53

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4L3

Tgt Ion: 95	Resp: 5784
Ion Ratio	Lower Upper
95 100	
97 67.1	44.7 83.1
132 99.8	66.6 123.6
130 94.0	66.5 123.5

