

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
 Data File : VU055314.D
 Acq On : 14 Sep 2023 18:29
 Operator : MD/SY
 Sample : 04380-01 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4F3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	109	rVB	67061	79676	14.14%	1.804%
2	1.907	185	192	207	rVB	67750	90083	15.99%	2.040%
3	2.563	384	396	409	rBV	91298	149643	26.56%	3.388%
4	3.042	531	545	559	rBV2	14756	27126	4.82%	0.614%
5	3.178	572	587	607	rVB2	10403	25242	4.48%	0.572%
6	4.634	1025	1040	1068	rBV	63853	199447	35.40%	4.516%
7	5.058	1157	1172	1193	rBV	91700	207686	36.87%	4.702%
8	5.721	1359	1378	1404	rBV3	179147	470400	83.50%	10.650%
9	6.248	1529	1542	1563	rBV	215950	420726	74.68%	9.526%
10	6.538	1620	1632	1649	rBV7	13476	29316	5.20%	0.664%
11	6.689	1661	1679	1696	rBV	110434	220510	39.14%	4.993%
12	7.566	1940	1952	1969	rBV2	48646	90141	16.00%	2.041%
13	7.898	2043	2055	2073	rBV	207419	365009	64.79%	8.264%
14	8.177	2133	2142	2157	rBV	28437	50811	9.02%	1.150%
15	8.634	2272	2284	2321	rBV5	173074	428005	75.98%	9.690%
16	9.415	2515	2527	2547	rBV	335593	563336	100.00%	12.754%
17	10.756	2932	2944	2962	rBV2	75672	128524	22.81%	2.910%
18	11.811	3259	3272	3291	rBV	341497	550724	97.76%	12.469%
19	12.190	3378	3390	3405	rBV	185843	314247	55.78%	7.115%
20	14.576	4123	4132	4140	rBV	4074	6113	1.09%	0.138%




Sum of corrected areas: 4416765

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
Data File : VU055314.D
Acq On : 14 Sep 2023 18:29
Operator : MD/SY
Sample : 04380-01 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4F3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

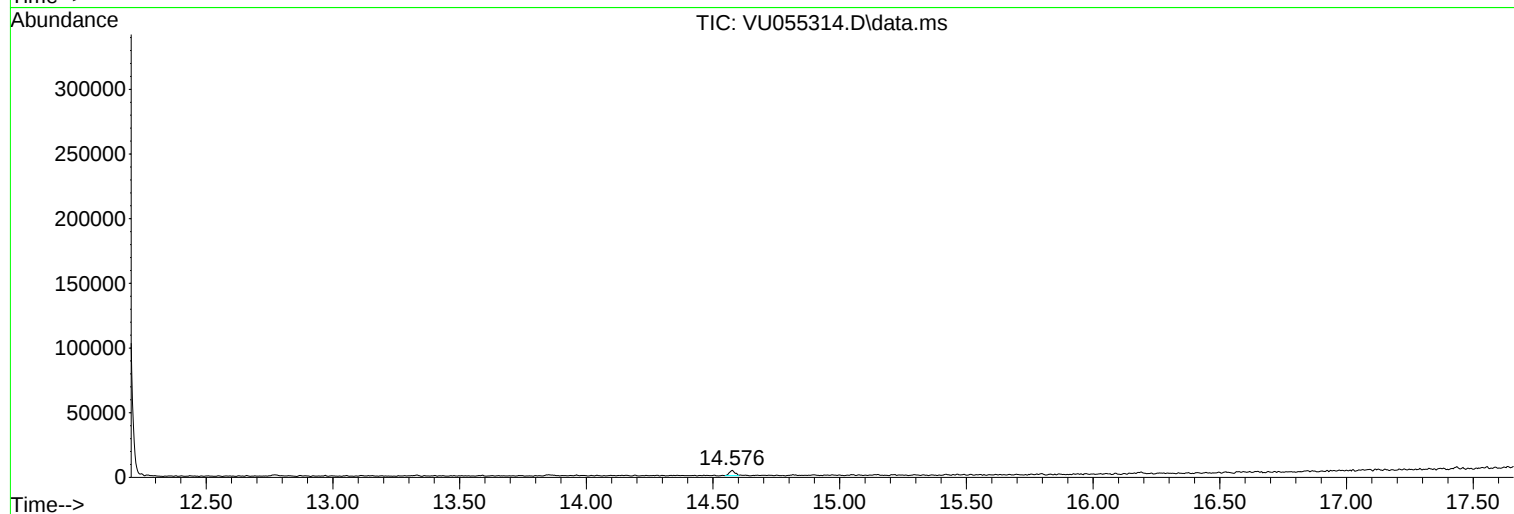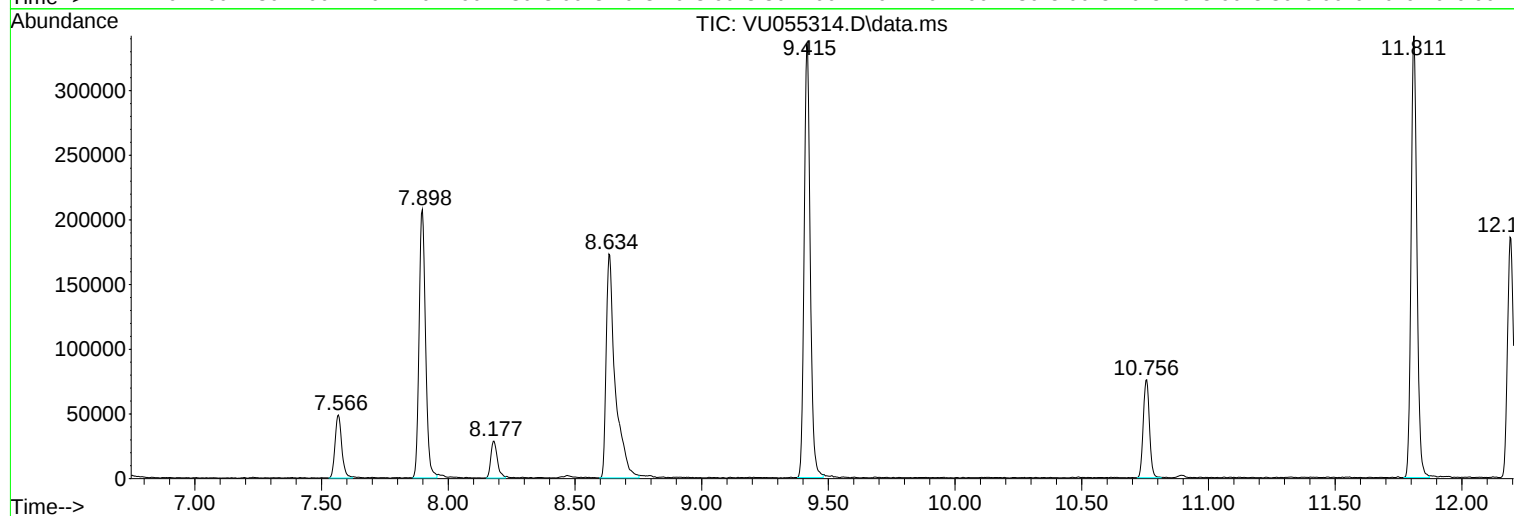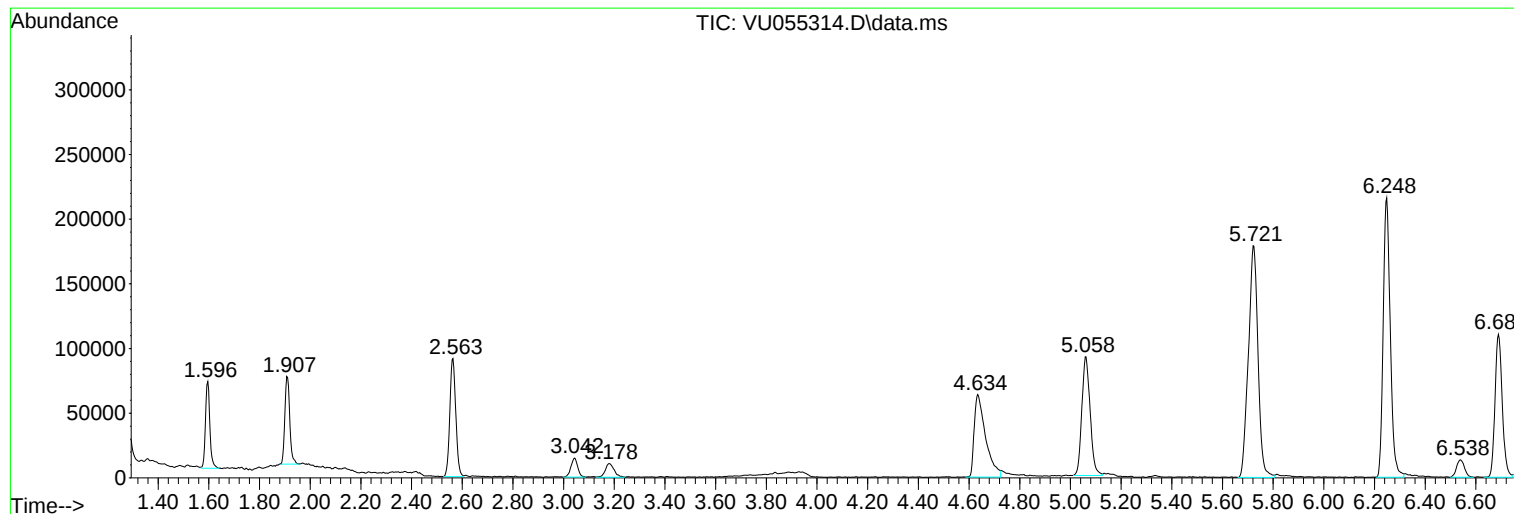

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
Data File : VU055314.D
Acq On : 14 Sep 2023 18:29
Operator : MD/SY
Sample : 04380-01 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4F3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
Data File : VU055314.D
Acq On : 14 Sep 2023 18:29
Operator : MD/SY
Sample : 04380-01 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4F3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc