

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
 Data File : VU055332.D
 Acq On : 15 Sep 2023 03:01
 Operator : MD/SY
 Sample : 04380-15 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4P9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055332.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	110	rVB2	164402	196340	13.49%	2.933%
2	1.911	184	193	205	rBV	68234	91279	6.27%	1.364%
3	2.564	381	396	414	rBV	93493	154258	10.60%	2.304%
4	3.043	531	545	559	rBV	18151	33708	2.32%	0.504%
5	3.184	574	589	604	rVB2	10293	22527	1.55%	0.337%
6	4.660	1022	1048	1072	rBV2	441965	1142737	78.52%	17.071%
7	5.059	1157	1172	1194	rBV	89649	200552	13.78%	2.996%
8	5.721	1358	1378	1409	rBV2	169505	448826	30.84%	6.705%
9	6.245	1529	1541	1562	rBV	194201	383029	26.32%	5.722%
10	6.538	1618	1632	1667	rBV	754972	1455403	100.00%	21.742%
11	6.689	1667	1679	1696	rVB	106156	210375	14.45%	3.143%
12	7.567	1939	1952	1967	rBV2	47237	86914	5.97%	1.298%
13	7.894	2042	2054	2072	rBV	206368	365903	25.14%	5.466%
14	8.177	2130	2142	2156	rBV3	26232	47860	3.29%	0.715%
15	8.634	2270	2284	2321	rBV3	150000	389291	26.75%	5.815%
16	9.415	2512	2527	2552	rBV	312822	531198	36.50%	7.935%
17	10.753	2930	2943	2957	rBV	72817	118831	8.16%	1.775%
18	11.811	3257	3272	3295	rBV	315932	512678	35.23%	7.659%
19	12.190	3378	3390	3408	rBV	180187	302386	20.78%	4.517%




Sum of corrected areas: 6694095

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
Data File : VU055332.D
Acq On : 15 Sep 2023 03:01
Operator : MD/SY
Sample : 04380-15 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4P9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

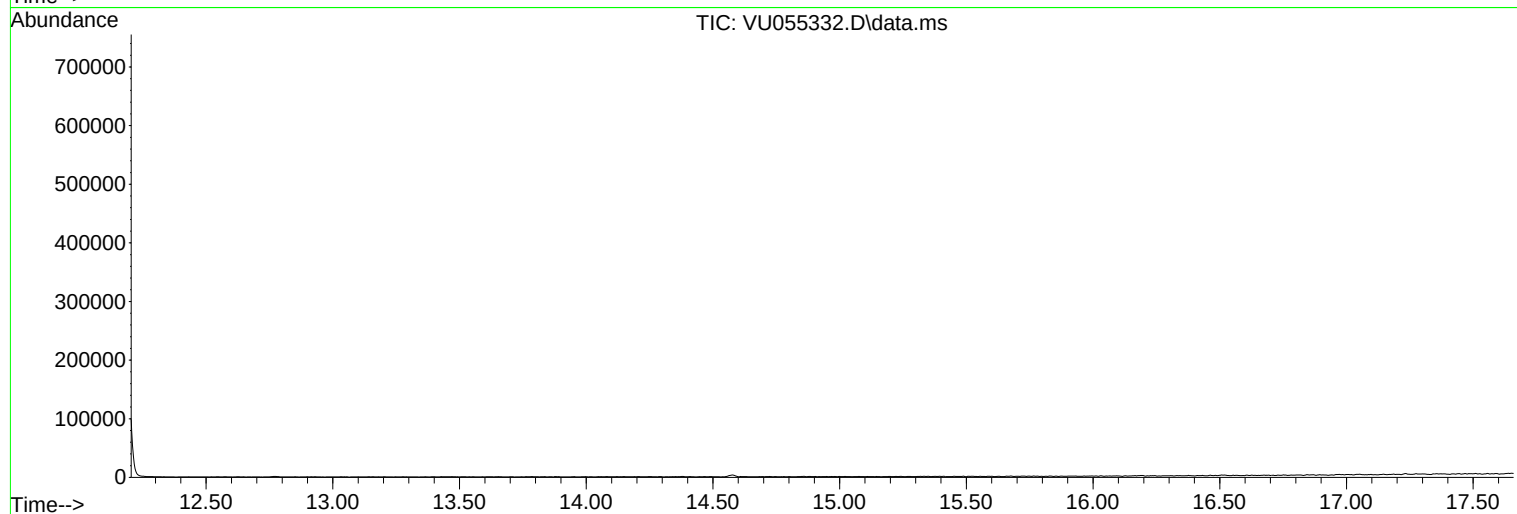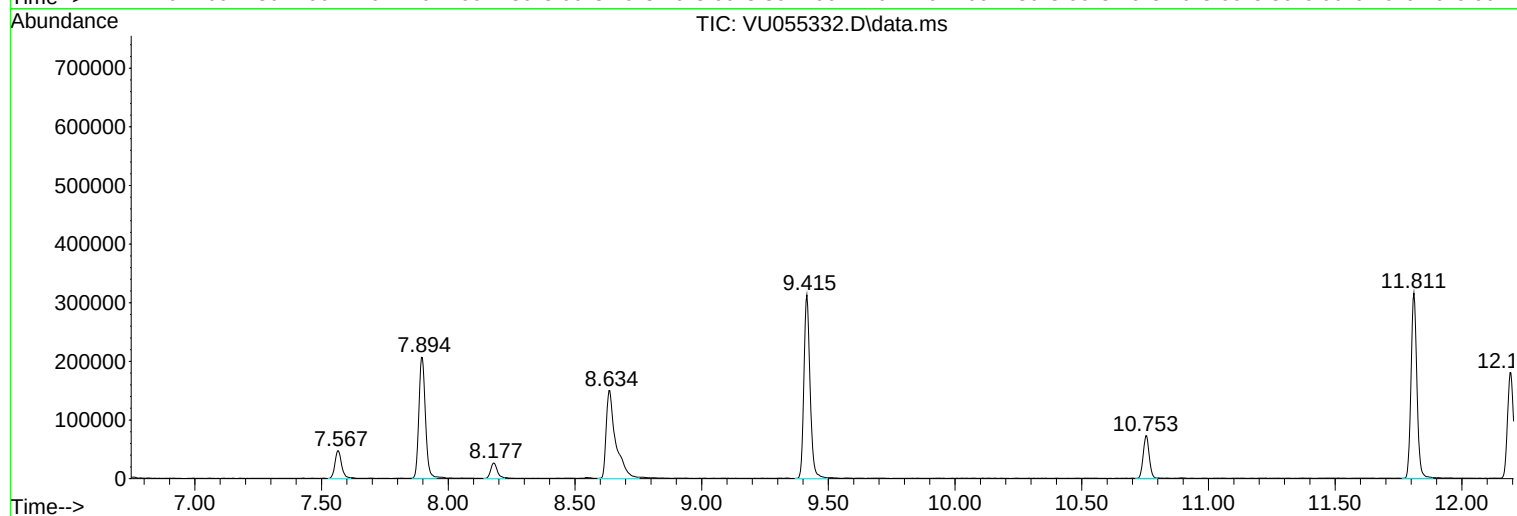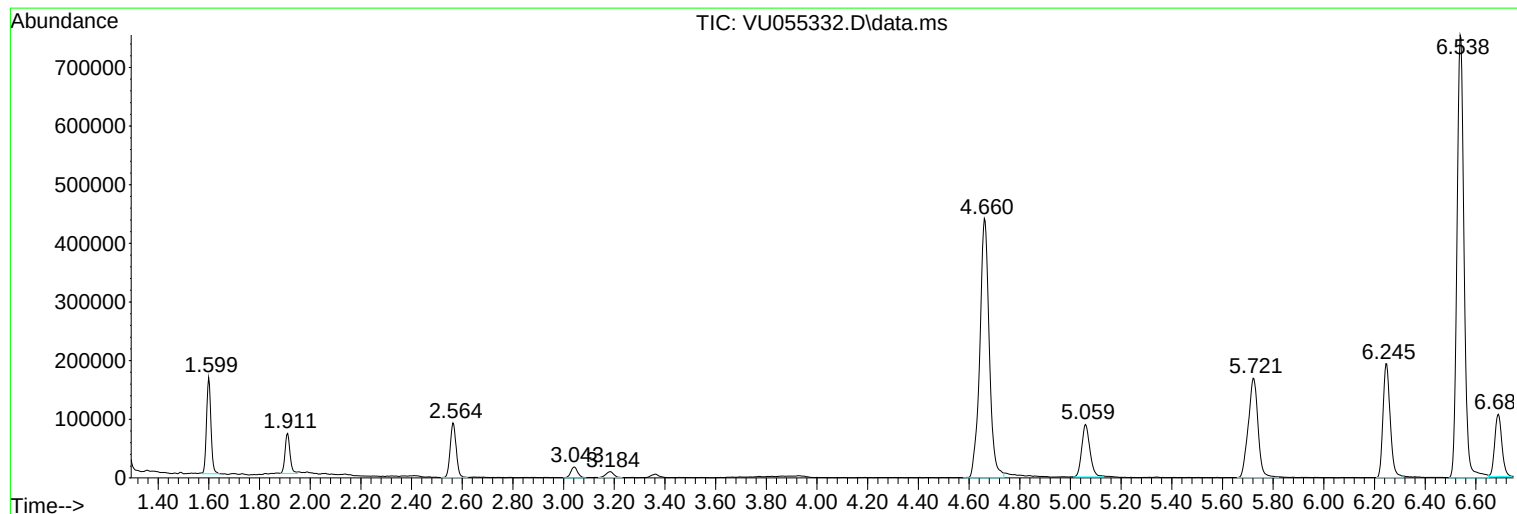

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
Data File : VU055332.D
Acq On : 15 Sep 2023 03:01
Operator : MD/SY
Sample : 04380-15 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4P9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
Data File : VU055332.D
Acq On : 15 Sep 2023 03:01
Operator : MD/SY
Sample : 04380-15 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4P9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc