


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091423\
Data File : VU055300.D
Acq On : 14 Sep 2023 08:47
Operator : MD/SY
Sample : BFB044
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB044

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Sep 15 02:53:52 2023

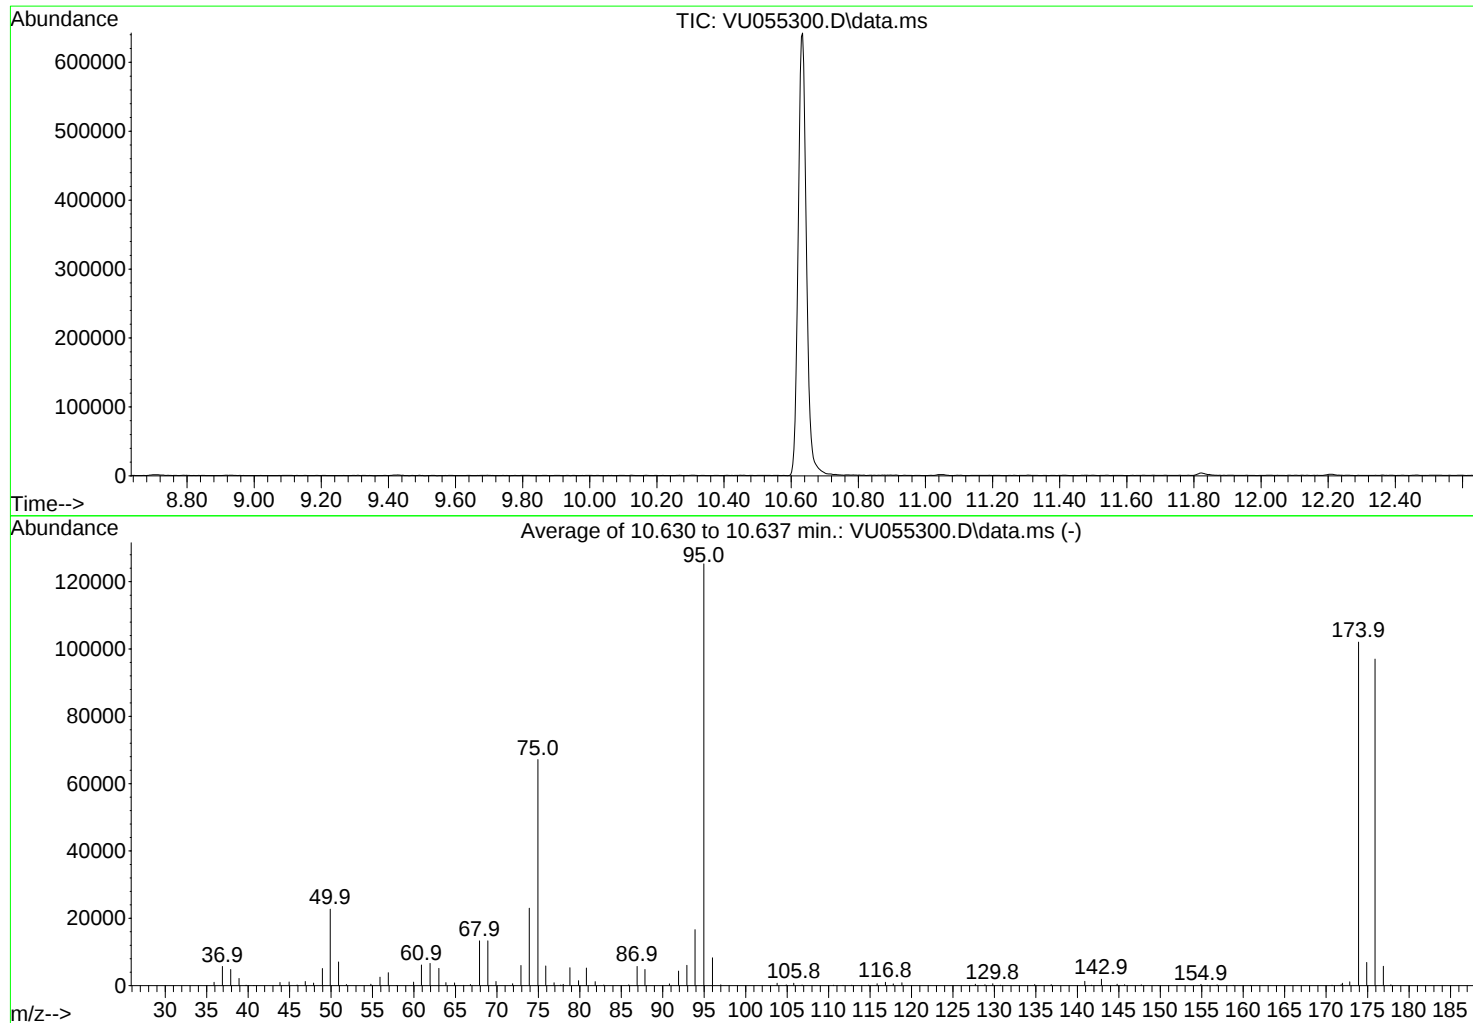

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	22731	PASS
75	95	30	80	53.6	67157	PASS
95	95	100	100	100.0	125307	PASS
96	95	5	9	6.6	8289	PASS
173	174	0.00	2	1.1	1134	PASS
174	95	50	120	81.5	102075	PASS
175	174	5	9	6.8	6906	PASS
176	174	95	101	95.0	96997	PASS
177	176	5	9	5.9	5755	PASS

m/z	Abundance
39.70	106.0
43.70	376.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	892.0
36.90	5824.0
37.90	5117.0
38.90	2281.0
39.80	226.0
40.70	103.0
43.90	1316.0
45.00	1207.0
45.90	206.0
47.00	1379.0
47.90	817.0
48.90	5208.0
49.90	23424.0
50.90	7341.0
51.80	361.0
54.80	361.0
55.90	2668.0
56.90	3879.0
59.90	1067.0
60.90	6607.0
61.90	7067.0
63.00	5243.0
63.90	994.0
64.90	765.0
66.80	271.0
67.90	13212.0
68.90	13645.0
69.90	1340.0
71.90	632.0
72.90	6345.0
73.90	23800.0
75.00	69688.0
75.90	6207.0
76.90	872.0
78.00	575.0
78.80	5615.0
79.80	1371.0
80.80	5318.0
81.90	1290.0
82.90	223.0
85.90	252.0
86.90	5783.0
87.90	4677.0
90.80	553.0
91.90	4603.0
92.90	6222.0
93.90	17288.0
95.00	127080.0
96.00	9227.0
97.00	214.0
103.80	692.0
104.90	276.0
105.80	708.0
106.80	186.0
110.60	126.0
111.80	126.0
112.80	237.0
114.90	166.0
115.90	540.0
116.90	1062.0
117.90	498.0
118.90	891.0
127.70	390.0
128.90	289.0
129.80	549.0
130.70	122.0
134.80	406.0
136.90	282.0
140.90	1330.0
141.60	138.0
142.90	1768.0
144.80	414.0
145.70	273.0
147.60	249.0
149.80	122.0
154.90	304.0
156.90	283.0
170.70	213.0
171.80	920.0
172.90	1234.0
173.90	102064.0
174.90	7289.0
175.90	96160.0
176.90	5953.0
177.80	208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	1031.0
36.90	5798.0
37.90	4842.0
38.90	2128.0
39.80	255.0
43.90	1408.0
45.00	1130.0
45.90	194.0
46.90	1296.0
47.90	797.0
49.00	5174.0
49.90	23152.0
50.90	7225.0
51.90	293.0
54.80	441.0
55.90	2590.0
56.90	3980.0
57.90	113.0
60.00	1012.0
60.90	6360.0
62.00	6855.0
63.00	5259.0
63.80	962.0
64.90	853.0
66.00	119.0
66.80	338.0
67.90	13692.0
68.90	13659.0
69.90	1220.0
71.90	572.0
72.90	6131.0
73.90	23856.0
74.90	68936.0
75.90	5874.0
76.90	933.0
78.00	535.0
78.80	5521.0
79.90	1521.0
80.80	5460.0
81.90	1220.0
82.90	200.0
85.90	251.0
86.90	6055.0
87.90	4866.0
90.80	503.0
91.90	4464.0
92.90	6205.0
93.90	17032.0
94.90	128384.0
96.00	8374.0
97.00	251.0
103.80	723.0
104.90	252.0
105.80	769.0
106.80	215.0
110.60	182.0
111.80	122.0
112.80	168.0
114.80	147.0
115.80	569.0
116.90	971.0
117.80	518.0
118.80	893.0
127.70	464.0
128.80	264.0
129.80	614.0
130.70	164.0
134.80	361.0
136.80	284.0
140.90	1310.0
141.70	161.0
142.90	1999.0
144.80	438.0
145.70	294.0
147.70	258.0
149.70	107.0
154.90	416.0
155.70	123.0
156.90	251.0
158.80	131.0
160.90	131.0
170.70	154.0
172.00	1023.0
172.90	1174.0
173.90	104888.0
174.90	7091.0
175.90	99544.0
176.90	5770.0
177.80	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	1064.0
36.90	5454.0
37.90	4436.0
38.90	1984.0
39.80	273.0
43.90	1317.0
44.90	987.0
45.90	160.0
46.80	1115.0
47.90	689.0
49.00	4879.0
49.90	21616.0
50.90	6589.0
51.90	297.0
54.80	476.0
55.90	2292.0
56.90	3648.0
57.90	122.0
60.00	992.0
60.90	5474.0
61.90	5936.0
63.00	4834.0
63.80	829.0
64.90	803.0
66.00	150.0
66.80	354.0
67.90	13063.0
68.90	12610.0
69.90	1100.0
71.90	483.0
72.90	5429.0
73.90	21384.0
74.90	62848.0
75.90	5437.0
76.90	746.0
77.70	549.0
78.80	4910.0
79.80	1493.0
80.80	4933.0
81.80	1115.0
82.90	173.0
85.90	196.0
86.90	5341.0
87.80	4840.0
90.80	484.0
91.90	3976.0
92.90	5625.0
93.90	15623.0
94.90	120456.0
96.00	7267.0
97.00	269.0
103.80	694.0
104.80	154.0
105.80	679.0
106.80	221.0
110.60	157.0
111.70	107.0
114.70	112.0
115.80	608.0
116.80	902.0
117.70	516.0
118.80	764.0
127.70	496.0
128.80	248.0
129.80	618.0
130.70	152.0
134.90	272.0
136.80	269.0
140.90	1230.0
141.80	148.0
142.90	1974.0
144.80	400.0
145.70	243.0
147.80	254.0
154.90	369.0
155.70	138.0
156.80	209.0
158.80	177.0
160.90	141.0
170.70	113.0
171.90	1074.0
172.80	995.0
173.90	99272.0
174.90	6339.0
175.90	95288.0
176.90	5542.0
177.80	233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044