

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091518\
 Data File : VU026731.D
 Acq On : 13 Sep 2018 17:30
 Operator : MD/SY
 Sample : J4893-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08K0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	63	70	81	rBV	94536	98673	16.17%	2.104%
2	1.678	150	157	174	rVB	69918	91181	14.94%	1.944%
3	2.273	331	342	355	rBV	152330	228751	37.49%	4.877%
4	2.395	377	380	384	rBV	188	162	0.03%	0.003%
5	2.443	386	395	404	rBV	6916	11433	1.87%	0.244%
6	2.624	443	451	455	rBV2	278	407	0.07%	0.009%
7	2.694	470	473	476	rVB2	200	114	0.02%	0.002%
8	2.717	477	480	482	rBV	302	210	0.03%	0.004%
9	2.823	509	513	515	rBV2	301	199	0.03%	0.004%
10	2.861	523	525	527	rBV	124	54	0.01%	0.001%
11	2.932	543	547	549	rBV	105	77	0.01%	0.002%
12	2.990	563	565	566	rBV	245	85	0.01%	0.002%
13	3.054	582	585	590	rVV	103	88	0.01%	0.002%
14	3.144	611	613	618	rVB	171	95	0.02%	0.002%
15	3.408	692	695	698	rBV	89	57	0.01%	0.001%
16	3.630	759	764	767	rBV	119	118	0.02%	0.003%
17	3.861	834	836	844	rVB2	215	246	0.04%	0.005%
18	3.900	844	848	851	rBV	120	116	0.02%	0.002%
19	4.003	877	880	883	rBV	84	53	0.01%	0.001%
20	4.128	916	919	920	rBV	64	41	0.01%	0.001%
21	4.180	920	935	961	rBV	52229	131654	21.58%	2.807%
22	4.376	994	996	1000	rBV2	140	133	0.02%	0.003%
23	4.398	1000	1003	1010	rVV3	363	384	0.06%	0.008%
24	4.479	1026	1028	1029	rBV3	129	34	0.01%	0.001%
25	4.591	1060	1063	1065	rBV	106	60	0.01%	0.001%
26	4.649	1065	1081	1103	rBV	102347	236723	38.80%	5.047%
27	4.749	1109	1112	1115	rBV2	193	113	0.02%	0.002%
28	4.855	1141	1145	1147	rBV	192	184	0.03%	0.004%
29	4.884	1152	1154	1161	rVB2	351	344	0.06%	0.007%
30	4.935	1167	1170	1175	rVB	126	84	0.01%	0.002%
31	4.961	1175	1178	1180	rBV	72	49	0.01%	0.001%
32	4.980	1181	1184	1185	rBV	68	36	0.01%	0.001%
33	5.006	1190	1192	1195	rVB2	153	86	0.01%	0.002%
34	5.193	1247	1250	1254	rBV	71	44	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091518\
 Data File : VU026731.D
 Acq On : 13 Sep 2018 17:30
 Operator : MD/SY
 Sample : J4893-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08K0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
 Title : VOC Analysis

35	5.250	1265	1268	1269	rBV	55	33	0.01%	0.001%
36	5.344	1273	1297	1326	rBV2	208886	610137	100.00%	13.008%
37	5.492	1338	1343	1346	rBV	92	96	0.02%	0.002%
38	5.511	1346	1349	1351	rVV	242	122	0.02%	0.003%
39	5.614	1377	1381	1384	rBV	62	47	0.01%	0.001%
40	5.630	1384	1386	1389	rBV	68	37	0.01%	0.001%
41	5.765	1423	1428	1432	rVB	142	121	0.02%	0.003%
42	5.787	1432	1435	1437	rBV	72	42	0.01%	0.001%
43	5.890	1451	1467	1494	rBV	206136	400802	65.69%	8.545%
44	6.180	1554	1557	1559	rBV	152	80	0.01%	0.002%
45	6.196	1559	1562	1564	rVB	246	108	0.02%	0.002%
46	6.218	1564	1569	1571	rBV	83	58	0.01%	0.001%
47	6.254	1577	1580	1586	rVB	70	62	0.01%	0.001%
48	6.334	1587	1605	1628	rVV	142781	279253	45.77%	5.953%
49	6.453	1641	1642	1644	rBV	120	63	0.01%	0.001%
50	6.537	1665	1668	1672	rVB	149	109	0.02%	0.002%
51	6.569	1672	1678	1684	rBV	177	197	0.03%	0.004%
52	6.633	1693	1698	1704	rVB	64	75	0.01%	0.002%
53	6.839	1757	1762	1763	rBV	59	46	0.01%	0.001%
54	6.855	1763	1767	1771	rBV	416	441	0.07%	0.009%
55	6.926	1786	1789	1791	rBV	71	51	0.01%	0.001%
56	7.006	1810	1814	1819	rBV	83	86	0.01%	0.002%
57	7.080	1833	1837	1841	rVB	89	70	0.01%	0.001%
58	7.102	1841	1844	1846	rBV	56	36	0.01%	0.001%
59	7.119	1846	1849	1853	rBV	53	45	0.01%	0.001%
60	7.231	1871	1884	1902	rBV	76878	133999	21.96%	2.857%
61	7.337	1914	1917	1918	rBV	151	86	0.01%	0.002%
62	7.373	1925	1928	1929	rBV	167	90	0.01%	0.002%
63	7.389	1929	1933	1943	rVV5	1417	2043	0.33%	0.044%
64	7.440	1946	1949	1952	rVB	95	66	0.01%	0.001%
65	7.463	1953	1956	1959	rVB	179	87	0.01%	0.002%
66	7.485	1959	1963	1965	rBV	203	124	0.02%	0.003%
67	7.498	1965	1967	1969	rVV	109	64	0.01%	0.001%
68	7.569	1975	1989	2008	rBV	281313	477829	78.32%	10.187%
69	7.723	2035	2037	2042	rVB2	199	137	0.02%	0.003%
70	7.758	2045	2048	2056	rVB	227	151	0.02%	0.003%
71	7.852	2066	2077	2096	rBV	53990	89396	14.65%	1.906%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091518\
 Data File : VU026731.D
 Acq On : 13 Sep 2018 17:30
 Operator : MD/SY
 Sample : J4893-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08K0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
 Title : VOC Analysis

72	8.086	2148	2150	2151	rVB	131	36	0.01%	0.001%
73	8.183	2167	2180	2191	rBV2	6099	13099	2.15%	0.279%
74	8.311	2210	2220	2248	rVB	171166	286334	46.93%	6.104%
75	8.553	2294	2295	2299	rBV	121	48	0.01%	0.001%
76	8.588	2304	2306	2308	rVB	139	38	0.01%	0.001%
77	8.713	2343	2345	2348	rBV	55	43	0.01%	0.001%
78	9.048	2446	2449	2450	rBV	114	62	0.01%	0.001%
79	9.093	2450	2463	2489	rVV	290954	474863	77.83%	10.124%
80	9.212	2499	2500	2502	rVB	247	50	0.01%	0.001%
81	9.257	2508	2514	2519	rBV2	252	378	0.06%	0.008%
82	9.305	2526	2529	2533	rVB	171	96	0.02%	0.002%
83	9.366	2546	2548	2549	rBV	127	52	0.01%	0.001%
84	9.376	2549	2551	2555	rBV2	209	204	0.03%	0.004%
85	9.665	2640	2641	2646	rVB	105	92	0.02%	0.002%
86	9.958	2730	2732	2735	rVB	140	58	0.01%	0.001%
87	9.999	2742	2745	2753	rVB	212	149	0.02%	0.003%
88	10.260	2821	2826	2828	rBV	161	152	0.02%	0.003%
89	10.353	2853	2855	2856	rBV	152	61	0.01%	0.001%
90	10.382	2862	2864	2866	rVB	171	70	0.01%	0.001%
91	10.434	2868	2880	2897	rBV	185580	292894	48.00%	6.244%
92	10.610	2925	2935	2948	rVB2	3889	6790	1.11%	0.145%
93	10.810	2994	2997	3003	rVB	229	158	0.03%	0.003%
94	10.852	3006	3010	3012	rBV2	161	95	0.02%	0.002%
95	10.999	3052	3056	3059	rBV	355	212	0.03%	0.005%
96	11.070	3076	3078	3080	rBV	141	48	0.01%	0.001%
97	11.485	3196	3207	3224	rBV	263915	409235	67.07%	8.725%
98	11.755	3283	3291	3300	rBV5	1378	1972	0.32%	0.042%
99	11.861	3312	3324	3341	rBV	253510	404883	66.36%	8.632%
100	12.321	3466	3467	3470	rVB	208	88	0.01%	0.002%


Sum of corrected areas: 4690637

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091518\
Data File : VU026731.D
Acq On : 13 Sep 2018 17:30
Operator : MD/SY
Sample : J4893-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08K0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

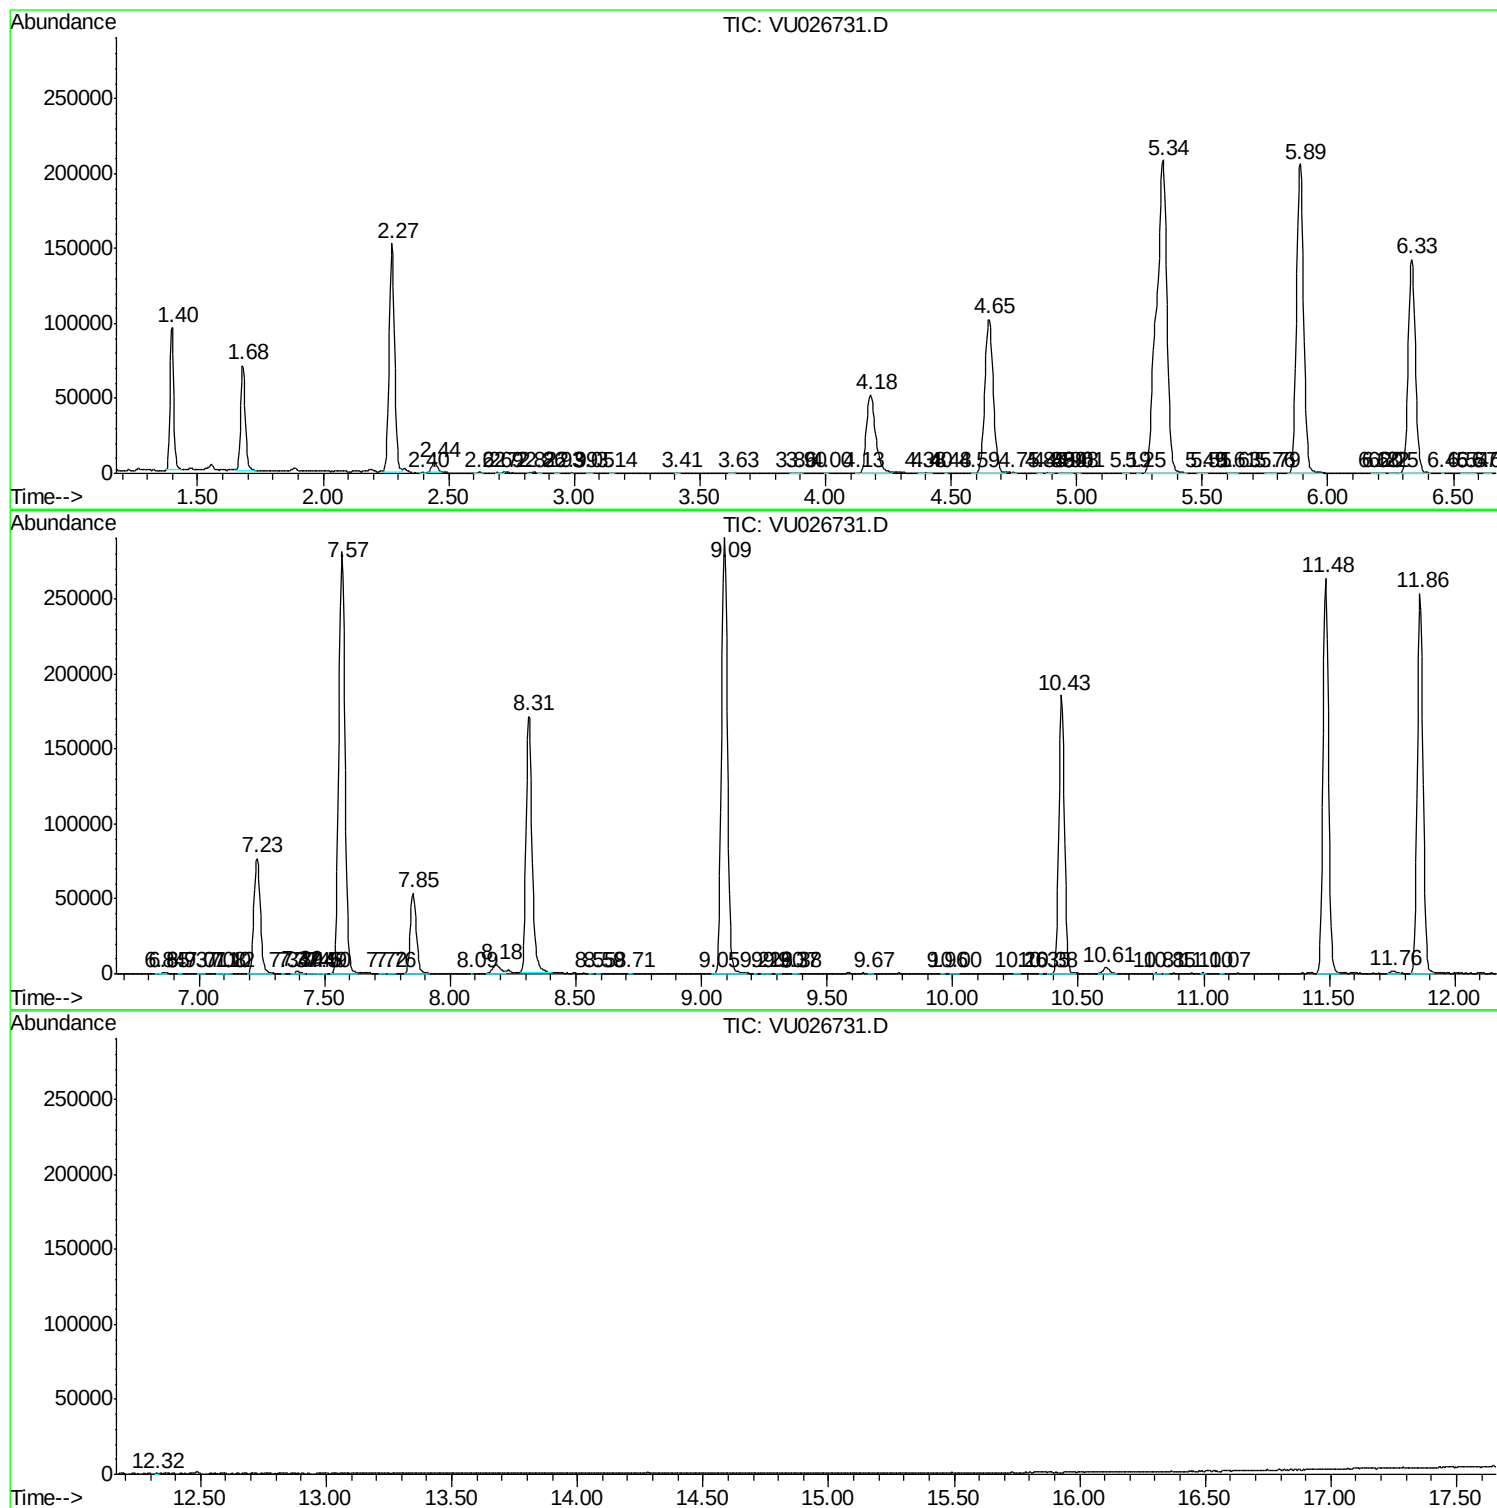

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091518\
Data File : VU026731.D
Acq On : 13 Sep 2018 17:30
Operator : MD/SY
Sample : J4893-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08K0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091518\
Data File : VU026731.D
Acq On : 13 Sep 2018 17:30
Operator : MD/SY
Sample : J4893-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08K0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc