


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091518\
Data File : VU026726.D
Acq On : 13 Sep 2018 13:53
Operator : MD/SY
Sample : BFB41
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
Title : VOC Analysis
Last Update : Sat Sep 15 00:18:06 2018

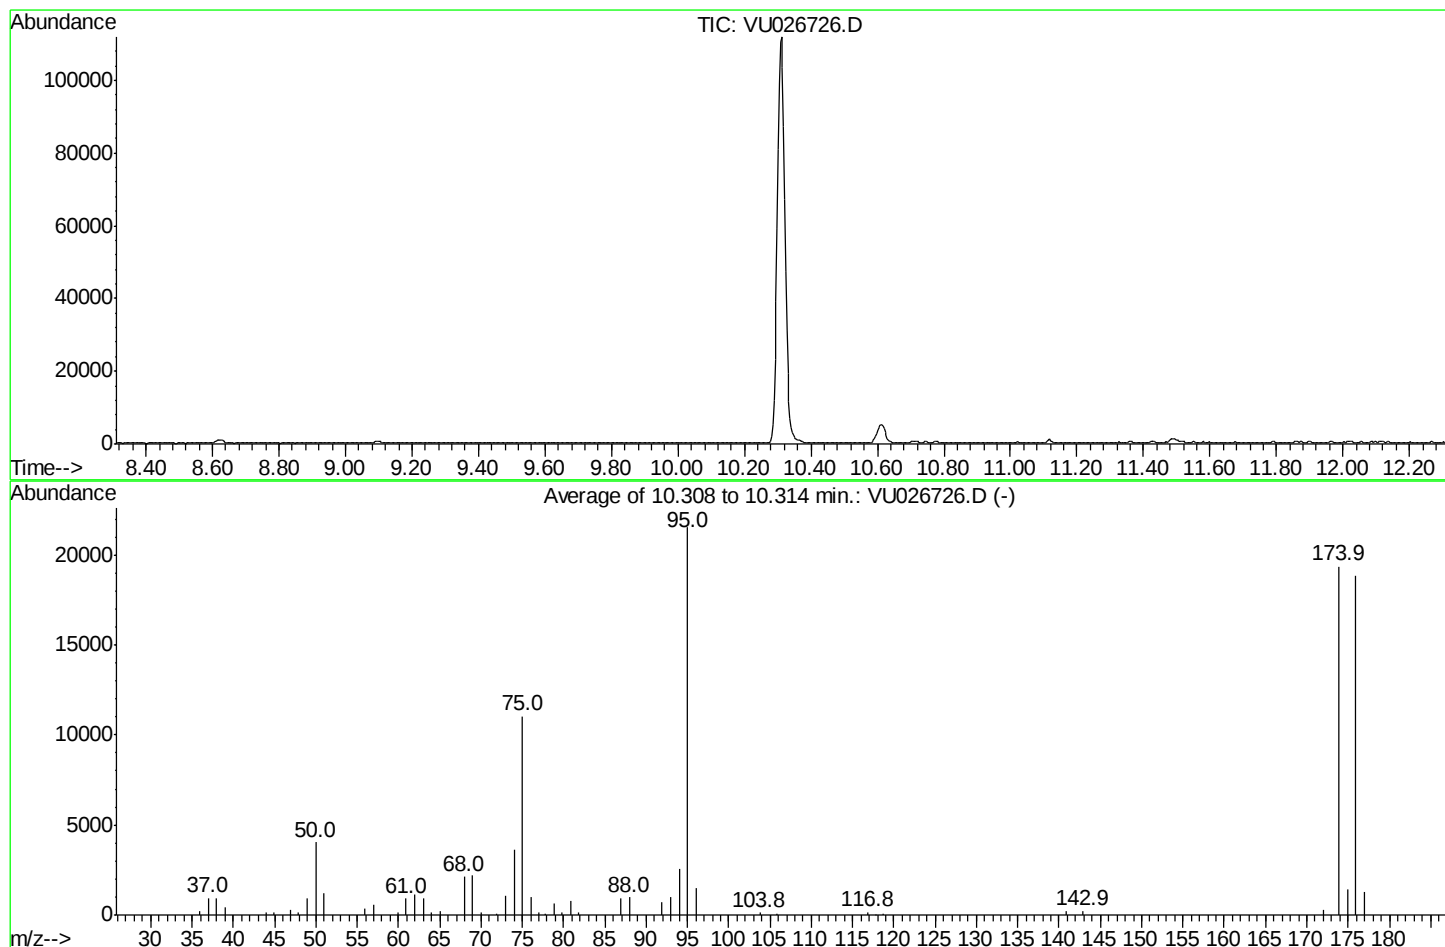

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	4033	PASS
75	95	30	80	51.2	11025	PASS
95	95	100	100	100.0	21530	PASS
96	95	5	9	7.0	1499	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.0	19368	PASS
175	174	5	9	7.3	1416	PASS
176	174	95	101	97.2	18826	PASS
177	176	5	9	6.7	1263	PASS