


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091518\
 Data File : VU026751.D
 Acq On : 14 Sep 2018 07:13
 Operator : MD/SY
 Sample : BFB42
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 15 00:18:06 2018

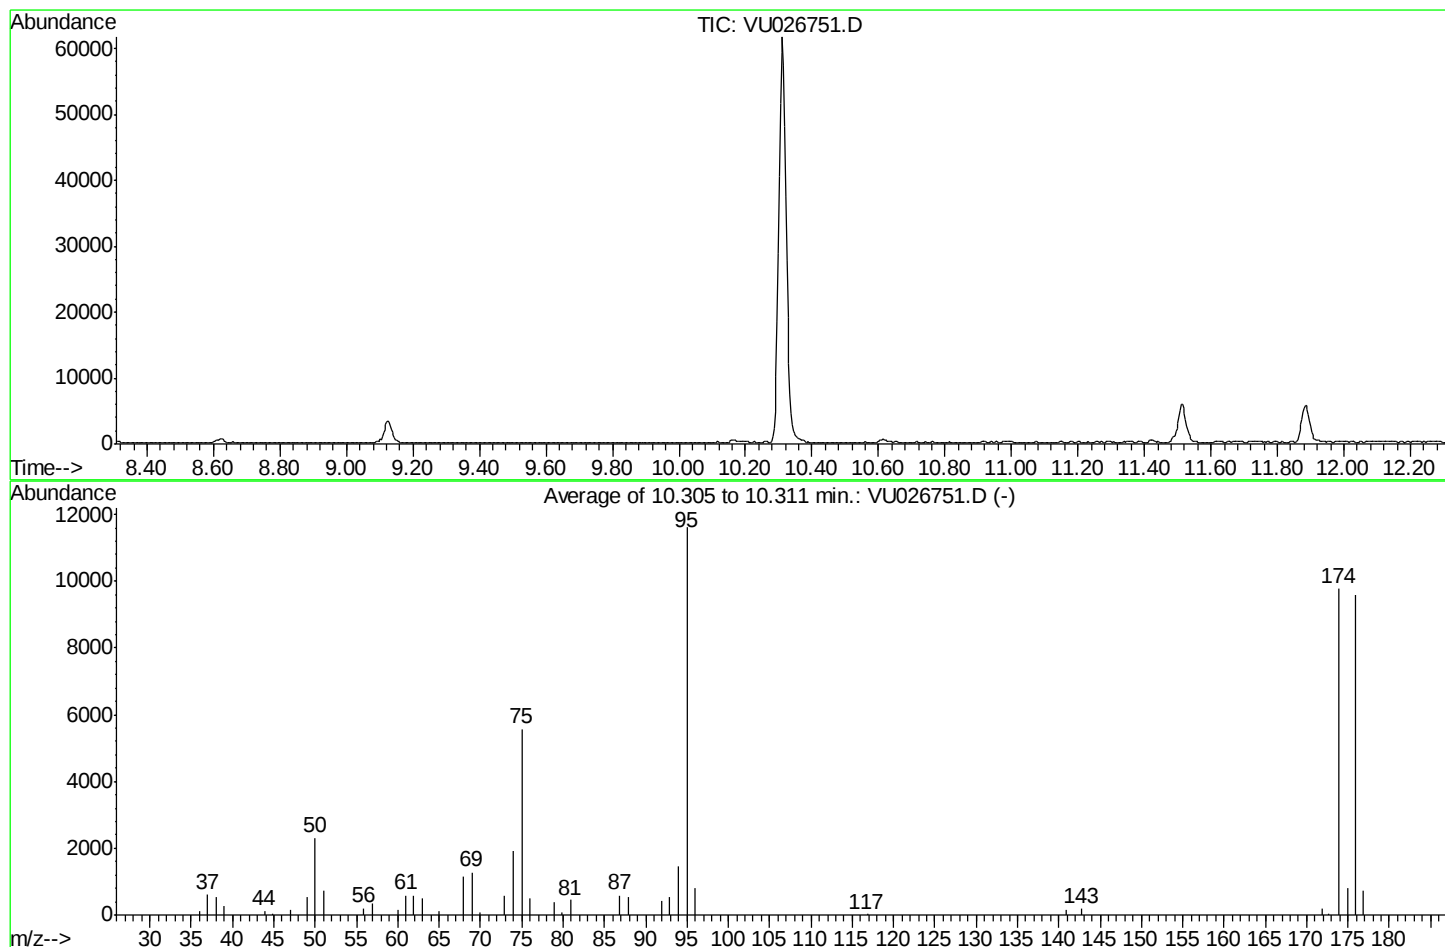

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	2304	PASS
75	95	30	80	48.0	5572	PASS
95	95	100	100	100.0	11614	PASS
96	95	5	9	6.9	806	PASS
173	174	0.00	2	0.4	41	PASS
174	95	50	120	84.2	9774	PASS
175	174	5	9	8.3	809	PASS
176	174	95	101	98.1	9587	PASS
177	176	5	9	7.7	739	PASS

m/z	Abundance
43.90	200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	119.0
37.00	506.0
38.00	490.0
39.00	225.0
44.00	288.0
47.00	151.0
49.00	503.0
50.00	2070.0
51.00	662.0
55.90	192.0
56.90	326.0
59.90	137.0
61.00	529.0
62.00	478.0
63.00	457.0
64.90	119.0
68.00	1128.0
68.90	1152.0
72.90	503.0
74.00	1722.0
75.00	5029.0
76.00	447.0
78.90	316.0
80.90	392.0
86.90	529.0
87.90	448.0
91.90	402.0
92.90	508.0
94.00	1227.0
95.00	10849.0
96.00	759.0
140.80	118.0
142.80	158.0
171.90	153.0
173.90	8545.0
174.90	671.0
175.90	8565.0
176.90	709.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	120.0
37.00	626.0
38.00	556.0
39.00	293.0
43.90	332.0
46.90	143.0
49.00	558.0
50.00	2384.0
51.00	725.0
55.90	213.0
56.90	368.0
60.00	161.0
61.00	604.0
61.90	577.0
63.00	497.0
65.00	124.0
68.00	1188.0
69.00	1317.0
70.00	100.0
72.90	601.0
74.00	1998.0
75.00	5714.0
76.00	497.0
78.90	381.0
79.90	126.0
80.90	466.0
86.90	619.0
87.90	556.0
91.90	423.0
92.90	564.0
94.00	1531.0
95.00	12024.0
96.00	830.0
140.90	150.0
142.80	199.0
171.90	206.0
173.90	10074.0
174.90	838.0
175.90	9876.0
176.90	768.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	128.0
37.00	681.0
38.00	586.0
39.00	338.0
43.90	362.0
44.80	100.0
46.90	126.0
49.00	524.0
50.00	2459.0
51.00	752.0
55.90	230.0
57.00	391.0
60.00	147.0
61.00	618.0
62.00	625.0
63.00	543.0
65.10	130.0
68.00	1153.0
69.00	1348.0
70.00	131.0
72.90	590.0
74.00	2072.0
75.00	5975.0
76.00	504.0
78.80	427.0
79.90	137.0
80.90	502.0
86.90	637.0
87.90	595.0
91.90	409.0
92.90	565.0
94.00	1620.0
95.00	11971.0
96.00	829.0
116.80	100.0
140.90	150.0
142.80	188.0
171.90	270.0
172.70	125.0
173.90	10705.0
174.90	920.0
175.90	10321.0
176.90	741.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42