


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091519\
 Data File : VU034548.D
 Acq On : 15 Sep 2019 07:06
 Operator : JC/SP
 Sample : BFB08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB08

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091519WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Sep 16 03:49:01 2019

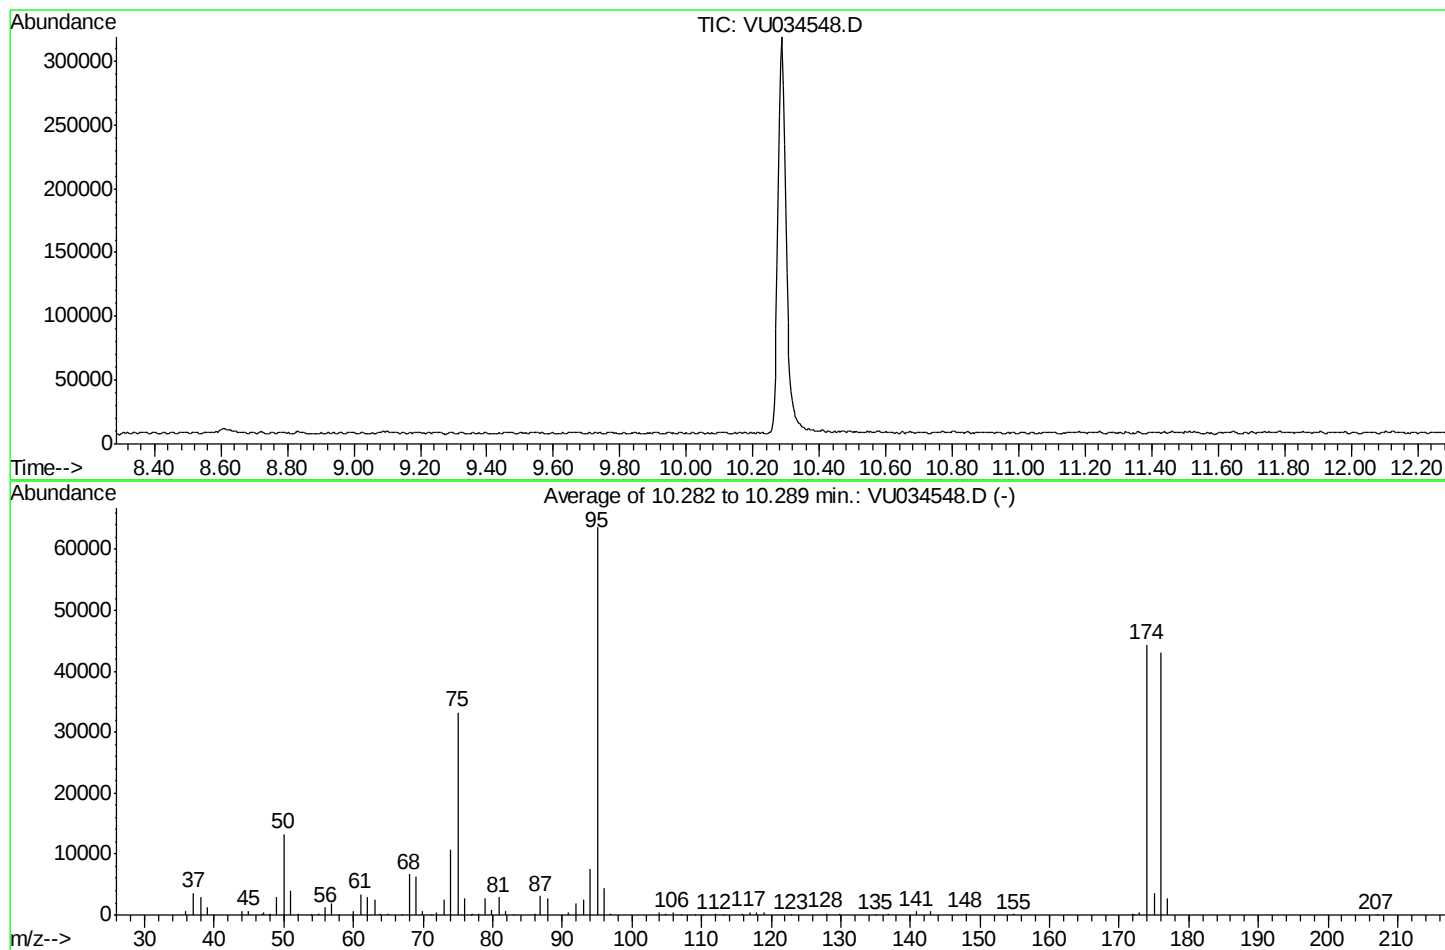

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	13263	PASS
75	95	30	80	52.2	33242	PASS
95	95	100	100	100.0	63629	PASS
96	95	5	9	6.8	4323	PASS
173	174	0.00	2	1.1	492	PASS
174	95	50	120	69.7	44370	PASS
175	174	5	9	8.0	3530	PASS
176	174	95	101	97.2	43117	PASS
177	176	5	9	6.5	2820	PASS

m/z	Abundance
36.00	713.0
37.00	3789.0
38.00	2816.0
39.00	1487.0
39.90	319.0
41.00	419.0
42.00	189.0
43.00	666.0
44.00	2082.0
44.90	837.0
46.90	703.0
47.80	330.0
49.00	2920.0
50.00	13274.0
51.00	4187.0
52.00	147.0
53.90	142.0
55.00	646.0
56.00	1277.0
56.90	2256.0
57.90	225.0
60.00	697.0
61.00	3197.0
62.00	2872.0
63.00	2419.0
63.90	295.0
64.90	117.0
67.00	302.0
68.00	6528.0
69.00	6587.0
69.90	753.0
71.20	186.0
71.90	354.0
73.00	2695.0
74.00	10558.0
75.00	33056.0
76.00	2795.0
77.10	397.0
78.00	309.0
78.90	2878.0
79.90	829.0
80.90	3116.0
81.90	731.0
83.00	306.0
84.90	131.0
86.10	172.0
86.90	3008.0
87.90	2673.0
90.90	424.0
91.90	1938.0
93.00	2564.0
94.00	7249.0
95.00	61800.0
96.00	4391.0
97.10	347.0
98.00	167.0
103.90	325.0
104.80	223.0
105.80	334.0
112.00	146.0
116.00	293.0
116.90	477.0
117.90	343.0
118.90	257.0
122.90	140.0
128.00	259.0
129.90	156.0
135.00	163.0
136.90	116.0
140.90	555.0
142.90	552.0
148.00	241.0
154.90	172.0
172.20	204.0
172.80	475.0
174.00	42176.0
175.00	3423.0
176.00	39872.0
177.00	2467.0
207.00	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
36.00	709.0
37.00	3785.0
38.00	3018.0
39.00	1626.0
39.90	298.0
41.00	456.0
41.90	111.0
43.00	614.0
44.00	2295.0
44.90	908.0
47.10	752.0
48.10	333.0
49.00	3036.0
50.00	13683.0
51.00	4214.0
52.00	179.0
52.90	103.0
53.90	129.0
55.00	674.0
56.00	1482.0
56.90	2193.0
57.90	218.0
60.00	789.0
61.00	3527.0
62.00	3002.0
63.00	2512.0
63.90	303.0
64.90	140.0
67.00	351.0
68.00	7034.0
69.00	6696.0
70.00	818.0
71.20	200.0
71.90	414.0
73.00	2853.0
74.00	10888.0
75.00	34272.0
76.00	2740.0
77.20	382.0
78.00	324.0
78.90	3024.0
79.90	916.0
80.90	3238.0
81.90	803.0
83.00	317.0
86.10	181.0
86.90	3213.0
87.90	2755.0
90.90	535.0
91.90	1983.0
93.00	2540.0
94.00	7868.0
95.00	65640.0
96.00	4549.0
97.10	376.0
98.00	176.0
103.90	326.0
104.90	185.0
105.90	378.0
107.00	112.0
110.10	112.0
112.00	156.0
113.10	118.0
115.90	304.0
116.90	504.0
117.90	345.0
118.90	344.0
122.90	136.0
128.00	263.0
129.90	167.0
135.00	149.0
136.90	152.0
140.90	660.0
143.00	595.0
148.00	224.0
154.90	210.0
171.90	189.0
172.90	511.0
174.00	45584.0
175.00	3652.0
176.00	44432.0
177.00	2928.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
35.00	592.0
37.00	3365.0
38.00	3096.0
39.00	1605.0
39.00	285.0
41.10	494.0
41.90	153.0
43.00	623.0
44.00	2336.0
44.90	925.0
47.10	717.0
48.10	400.0
49.00	3060.0
50.00	12833.0
51.00	4020.0
52.00	185.0
52.90	110.0
55.00	662.0
56.00	1542.0
57.00	2221.0
57.90	195.0
60.00	855.0
61.00	3516.0
62.00	2925.0
63.00	2413.0
63.90	267.0
64.90	137.0
67.00	351.0
68.00	6943.0
69.00	6380.0
70.00	845.0
71.20	228.0
71.90	398.0
73.00	2772.0
74.00	10448.0
75.00	32400.0
76.00	2476.0
76.90	373.0
78.00	279.0
78.90	2832.0
79.90	880.0
80.90	3017.0
81.90	710.0
83.00	288.0
86.10	133.0
86.90	3167.0
87.90	2820.0
90.90	542.0
91.90	1885.0
93.00	2428.0
94.00	7648.0
95.00	63448.0
96.10	4349.0
97.00	392.0
98.10	164.0
104.00	328.0
105.00	174.0
105.90	366.0
107.00	135.0
109.00	118.0
112.00	136.0
115.90	255.0
116.90	488.0
117.90	340.0
118.90	390.0
127.90	249.0
129.90	205.0
136.90	125.0
140.90	581.0
143.00	609.0
147.90	173.0
154.90	226.0
171.90	157.0
173.00	491.0
174.00	45352.0
175.00	3516.0
176.00	45048.0
177.00	3067.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
38.90	352.0
39.90	273.0
40.90	586.0
42.00	258.0
42.90	883.0
43.90	1554.0
44.90	164.0
51.00	116.0
53.10	134.0
55.00	532.0
56.10	247.0
56.90	380.0
57.80	145.0
59.90	179.0
66.90	287.0
68.00	193.0
69.10	310.0
70.10	155.0
71.00	121.0
73.00	168.0
77.00	110.0
79.00	125.0
80.90	202.0
82.10	119.0
82.90	291.0
84.00	263.0
84.90	102.0
91.00	151.0
96.10	106.0
96.90	168.0
98.00	228.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08