

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091520\
 Data File : VU040135.D
 Acq On : 15 Sep 2020 13:02
 Operator : SY/MD
 Sample : VU0915WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK06

Quant Time: Sep 16 03:16:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 16 03:11:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	109979	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	115254	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	49902	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	32717	5.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.00%
7) Chloroethane-d5	1.92	69	28378	5.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.40%
11) 1,1-Dichloroethene-d2	2.58	63	54421	3.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.60%
20) 2-Butanone-d5	4.66	46	122709	51.09	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.18%
24) Chloroform-d	5.08	84	63981	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.20%
26) 1,2-Dichloroethane-d4	5.72	65	41149	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
32) Benzene-d6	5.74	84	123776	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
36) 1,2-Dichloropropane-d6	6.70	67	39275	4.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.60%
41) Toluene-d8	7.90	98	99134	4.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.60%
43) trans-1,3-Dichloropropene-	8.19	79	16231	3.98	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.60%
46) 2-Hexanone-d5	8.64	63	85024	44.06	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.12%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	36470	4.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	38668	4.79	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.80%


Target Compounds					Ovalue
16) Methylene chloride	3.05	84	1766	0.158 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091520\
Data File : VU040135.D
Acq On : 15 Sep 2020 13:02
Operator : SY/MD
Sample : VU0915WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK06

Quant Time: Sep 16 03:16:37 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Sep 16 03:11:25 2020
Response via : Initial Calibration

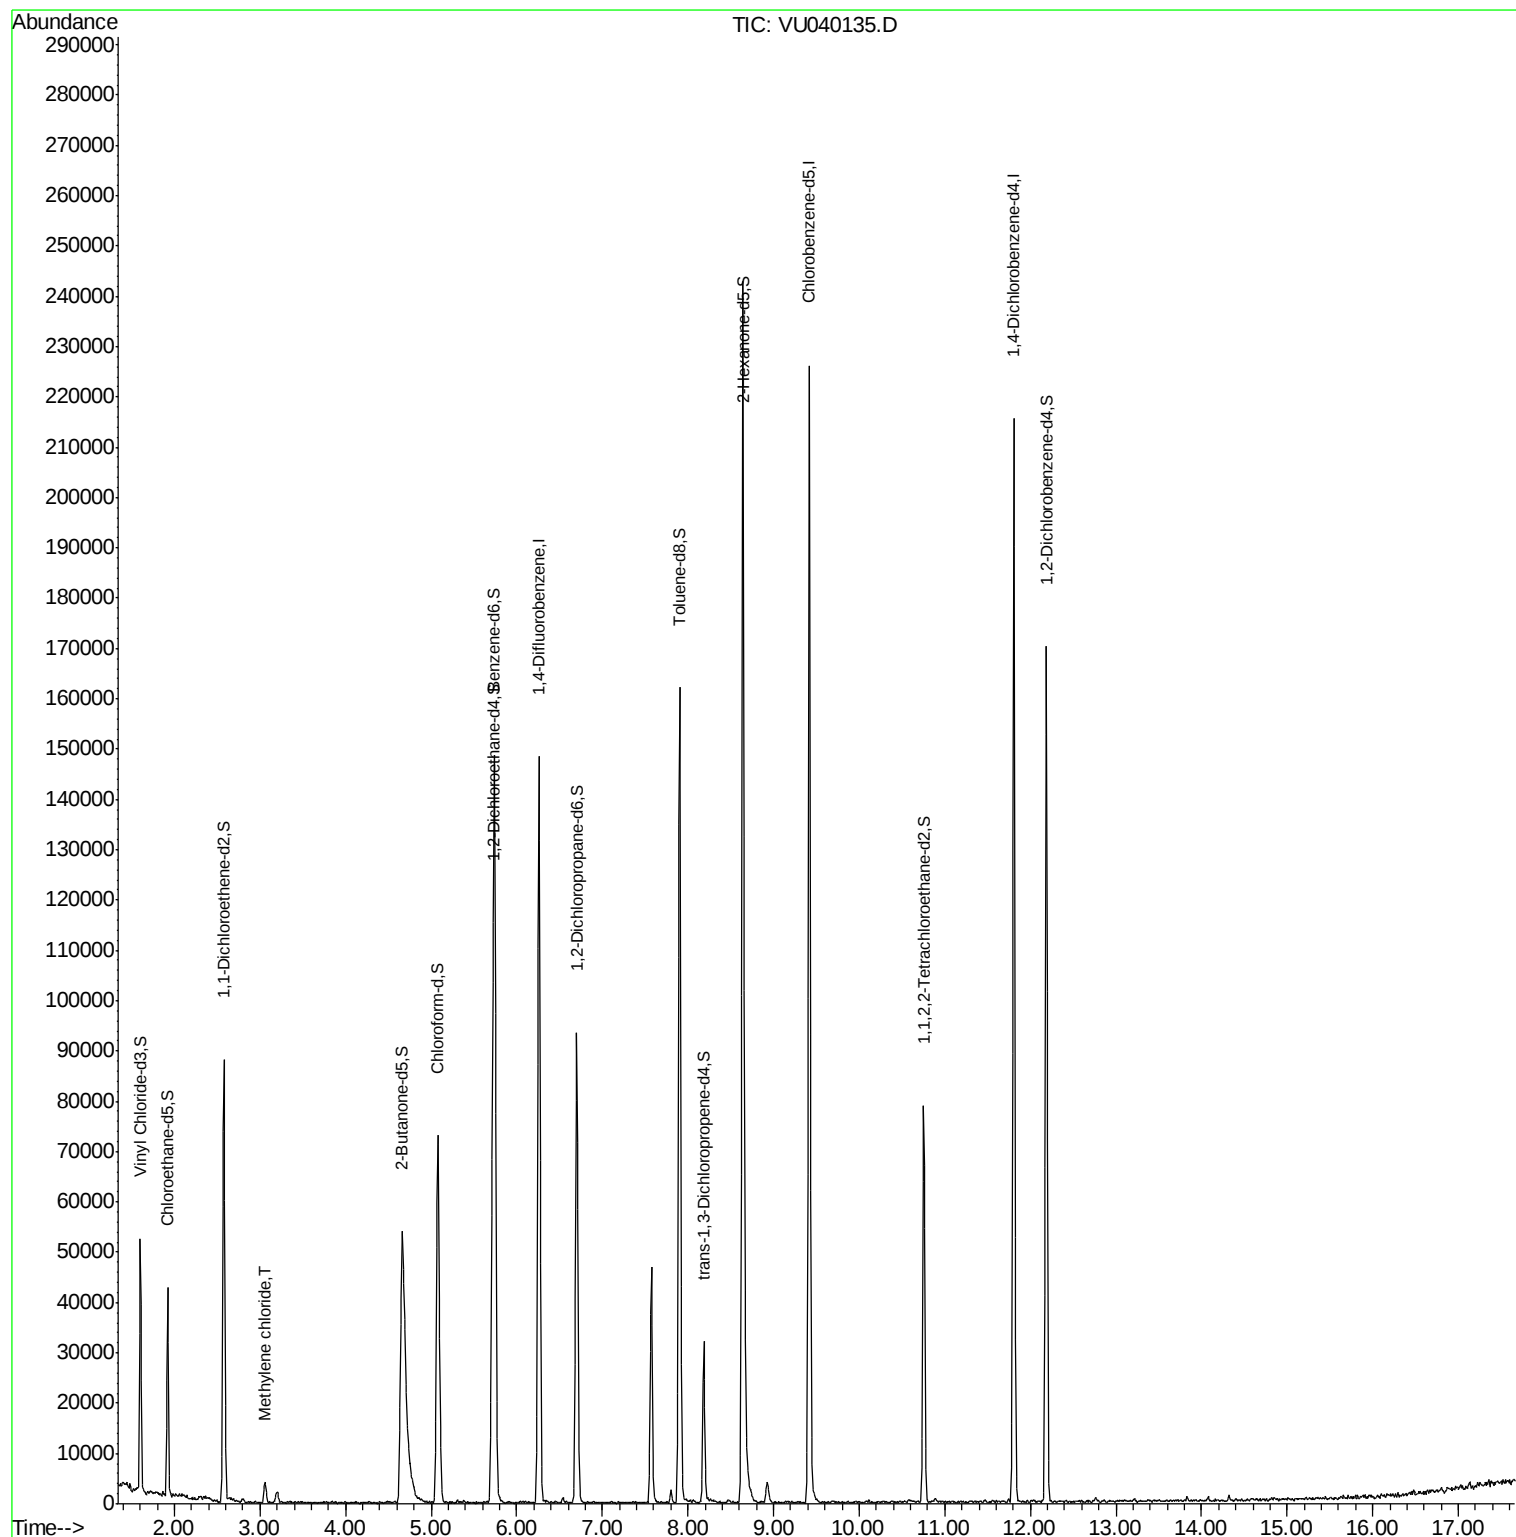

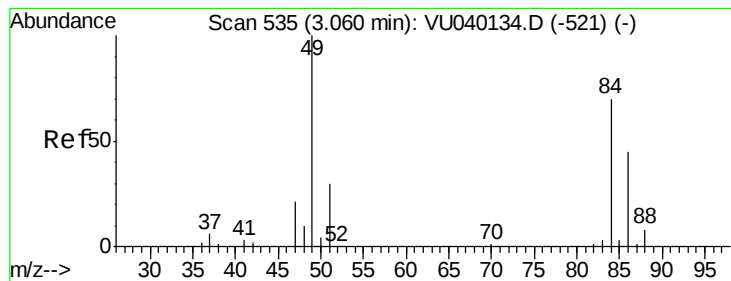

#16
 Methvlene chloride
 Concen: 0.158 ug/L
 RT: 3.05 min Scan# 533
 Delta R.T. -0.01 min
 Lab File: VU040135.D
 Acq: 15 Sep 2020 13:02

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK06

Tot Ion: 84 Resp: 1766
 Ion Ratio Lower Upper
 84 100
 86 74.7 45.2 84.0
 49 158.0 104.0 193.2

