


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091520\
 Data File : VU040133.D
 Acq On : 15 Sep 2020 10:44
 Operator : SY/MD
 Sample : BFB01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB01

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Sep 16 03:11:25 2020

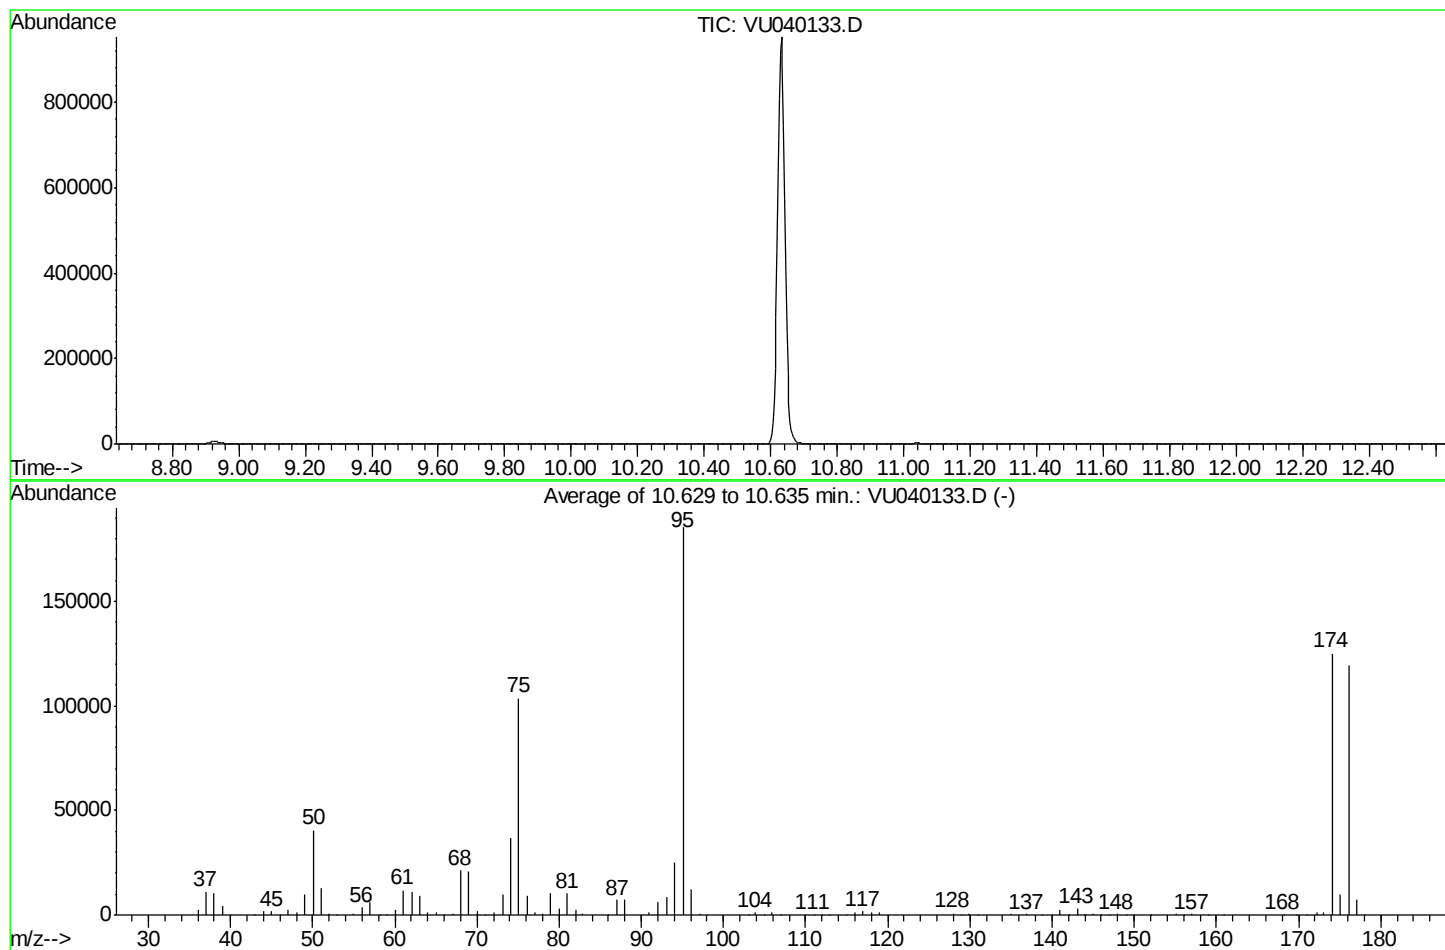

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	40626	PASS
75	95	30	80	55.9	103677	PASS
95	95	100	100	100.0	185344	PASS
96	95	5	9	6.7	12467	PASS
173	174	0.00	2	0.9	1184	PASS
174	95	50	120	67.4	124914	PASS
175	174	5	9	7.9	9825	PASS
176	174	95	101	95.7	119573	PASS
177	176	5	9	6.3	7571	PASS

m/z	Abundance
36.10	2337.0
37.00	11859.0
38.00	10859.0
39.10	4086.0
40.00	205.0
43.00	141.0
44.10	1712.0
45.00	1852.0
46.10	316.0
47.10	2283.0
48.00	1605.0
49.00	10284.0
50.10	42096.0
51.10	12558.0
52.00	550.0
52.90	119.0
55.00	629.0
56.00	3742.0
57.00	6524.0
58.20	312.0
60.00	2350.0
61.00	11868.0
62.10	11304.0
63.10	9567.0
64.00	1098.0
65.00	1640.0
66.00	158.0
67.10	662.0
68.00	21192.0
69.00	21664.0
70.10	1652.0
71.10	122.0
72.10	1390.0
73.10	9965.0
74.10	37504.0
75.10	103824.0
76.10	8971.0
77.10	1155.0
78.10	820.0
79.00	10707.0
80.00	2786.0
81.00	10183.0
82.00	2180.0
82.90	352.0
86.10	236.0
87.00	7536.0
88.00	6848.0
91.00	1004.0
92.00	6076.0
93.00	8581.0
94.10	24872.0
95.10	187328.0
96.10	12801.0
97.10	456.0
103.10	195.0
103.90	1149.0
105.00	268.0
105.90	1066.0
106.90	207.0
109.90	152.0
111.00	312.0
111.90	162.0
112.90	324.0
114.90	204.0
115.90	1012.0
117.00	1684.0
118.00	1004.0
118.90	1392.0
128.00	854.0
128.90	232.0
129.90	576.0
131.00	258.0
135.00	309.0
136.90	457.0
138.70	128.0
140.00	127.0
141.00	2213.0
142.00	327.0
143.10	2845.0
143.90	220.0
145.00	583.0
146.00	264.0
147.10	185.0
147.90	496.0
150.00	251.0
155.10	359.0
157.00	457.0
158.90	183.0
161.00	227.0
169.70	106.0
171.10	243.0
172.20	1315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

173.00	1771.0
174.10	121576.0
175.10	10035.0
176.10	117112.0
177.10	7325.0
178.00	257.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.10	2393.0
37.00	11557.0
38.00	11121.0
39.10	4174.0
39.90	231.0
42.80	121.0
44.10	1935.0
45.00	1840.0
46.00	305.0
47.00	2233.0
48.00	1518.0
49.00	10450.0
50.10	41704.0
51.10	12998.0
52.00	496.0
52.90	137.0
55.00	650.0
56.00	3798.0
57.00	6559.0
58.20	294.0
60.00	2466.0
61.00	12311.0
62.10	11434.0
63.10	9848.0
64.00	1064.0
65.10	1417.0
67.00	576.0
68.00	22048.0
69.00	21672.0
70.00	1597.0
71.00	106.0
72.10	1260.0
73.10	10322.0
74.10	37520.0
75.10	107064.0
76.10	9254.0
77.10	1199.0
78.00	802.0
78.90	10956.0
80.00	3031.0
81.00	10606.0
82.00	2347.0
82.80	343.0
85.90	206.0
87.00	7340.0
88.00	7381.0
91.00	979.0
92.10	6405.0
93.00	8989.0
94.10	26232.0
95.10	191936.0
96.10	12936.0
97.10	375.0
103.10	155.0
103.90	1234.0
105.00	279.0
105.90	1105.0
106.90	226.0
109.90	193.0
111.00	313.0
111.90	261.0
112.90	331.0
115.00	211.0
116.00	944.0
117.00	1672.0
118.00	1082.0
118.90	1408.0
128.00	952.0
128.90	239.0
129.90	627.0
131.00	310.0
135.00	378.0
136.90	455.0
138.80	106.0
139.90	167.0
141.00	2296.0
142.10	332.0
143.00	2847.0
143.90	168.0
145.00	430.0
146.00	306.0
147.00	153.0
147.90	525.0
149.10	133.0
150.00	225.0
152.00	112.0
155.10	365.0
156.10	101.0
157.00	416.0
159.00	241.0
160.90	233.0
168.20	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

169.70	119.0
171.00	228.0
172.20	1398.0
173.10	1782.0
174.10	129528.0
175.10	10138.0
176.10	123520.0
177.10	7811.0
178.00	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.10	2111.0
37.00	10564.0
38.00	10156.0
39.10	3853.0
39.90	250.0
42.80	129.0
44.00	1923.0
45.00	1695.0
46.00	231.0
47.00	2069.0
48.00	1356.0
49.00	9097.0
50.10	38080.0
51.10	12195.0
52.00	408.0
53.00	119.0
55.00	525.0
56.00	3435.0
57.00	6128.0
58.10	253.0
58.90	133.0
60.00	2316.0
61.00	11014.0
62.10	10231.0
63.10	8936.0
64.00	922.0
65.10	1089.0
67.00	454.0
68.00	20328.0
69.00	19976.0
70.00	1416.0
72.10	1046.0
73.10	9827.0
74.10	34336.0
75.10	100144.0
76.10	8534.0
77.00	1101.0
78.00	698.0
78.90	10111.0
80.00	2834.0
81.00	10175.0
82.00	2308.0
82.90	308.0
85.90	147.0
87.10	6854.0
88.00	7092.0
90.90	897.0
92.10	5895.0
93.10	8477.0
94.10	24440.0
95.10	176768.0
96.10	11666.0
97.10	299.0
103.90	1202.0
105.00	284.0
106.00	1008.0
106.90	210.0
109.80	203.0
111.00	247.0
111.90	274.0
112.90	278.0
115.00	218.0
116.00	977.0
117.00	1549.0
118.00	992.0
118.90	1346.0
128.00	845.0
128.90	231.0
130.00	690.0
131.00	299.0
135.00	436.0
136.90	412.0
139.90	206.0
141.00	2289.0
142.10	270.0
143.00	2716.0
144.10	125.0
145.00	333.0
145.90	329.0
147.90	440.0
149.10	169.0
150.00	216.0
155.00	348.0
156.10	122.0
157.00	356.0
159.00	291.0
160.90	189.0
168.20	124.0
170.90	199.0
172.20	1167.0
174.10	123640.0
175.10	9303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

176.10

177.10

178.00

118088.0

7578.0

226.0

Instrument :

MSVOA_U

ClientSampleId :

BFB01

Scan 2875 (10.584 min): VU040133.D
BFB01

m/z	Abundance
39.90	145.0
43.90	277.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01