

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091521\
 Data File : VU044638.D
 Acq On : 15 Sep 2021 12:16
 Operator : SY/MD
 Sample : VU0915WBL04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK020

Manual Integrations
 APPROVED

MMDadoda
 9/16/2021 12:12:48 PM

Quant Time: Sep 16 01:42:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 16 01:40:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	138067	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	142254	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	66758	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	31327	3.845	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.000%
7) Chloroethane-d5	1.919	69	34407	4.139	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.800%
11) 1,1-Dichloroethene-d2	2.575	65	17011	4.134	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.600%
20) 2-Butanone-d5	4.645	46	160863m	47.105	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.220%
24) Chloroform-d	5.073	84	73659	4.299	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
26) 1,2-Dichloroethane-d4	5.710	65	46333	4.535	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.600%
32) Benzene-d6	5.735	84	149869	4.132	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.600%
36) 1,2-Dichloropropane-d6	6.700	67	52700	4.424	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.400%
41) Toluene-d8	7.906	98	123007	3.895	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.000%
43) trans-1,3-Dichloroprop...	8.185	79	16616	3.957	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.200%
46) 2-Hexanone-d5	8.648	63	117882	43.681	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.360%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	45426	4.301	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.000%
66) 1,2-Dichlorobenzene-d4	12.198	152	47787	4.338	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.800%
Target Compounds						Qvalue
16) Methylene chloride	3.054	84	5257	0.373	ug/L	85
25) Chloroform	5.102	83	5097	0.251	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091521\
Data File : VU044638.D
Acq On : 15 Sep 2021 12:16
Operator : SY/MD
Sample : VU0915WBL04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
VBLK020

Manual Integrations
APPROVED

MMDadoda
9/16/2021 12:12:48 PM


Quant Time: Sep 16 01:42:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 16 01:40:15 2021
Response via : Initial Calibration

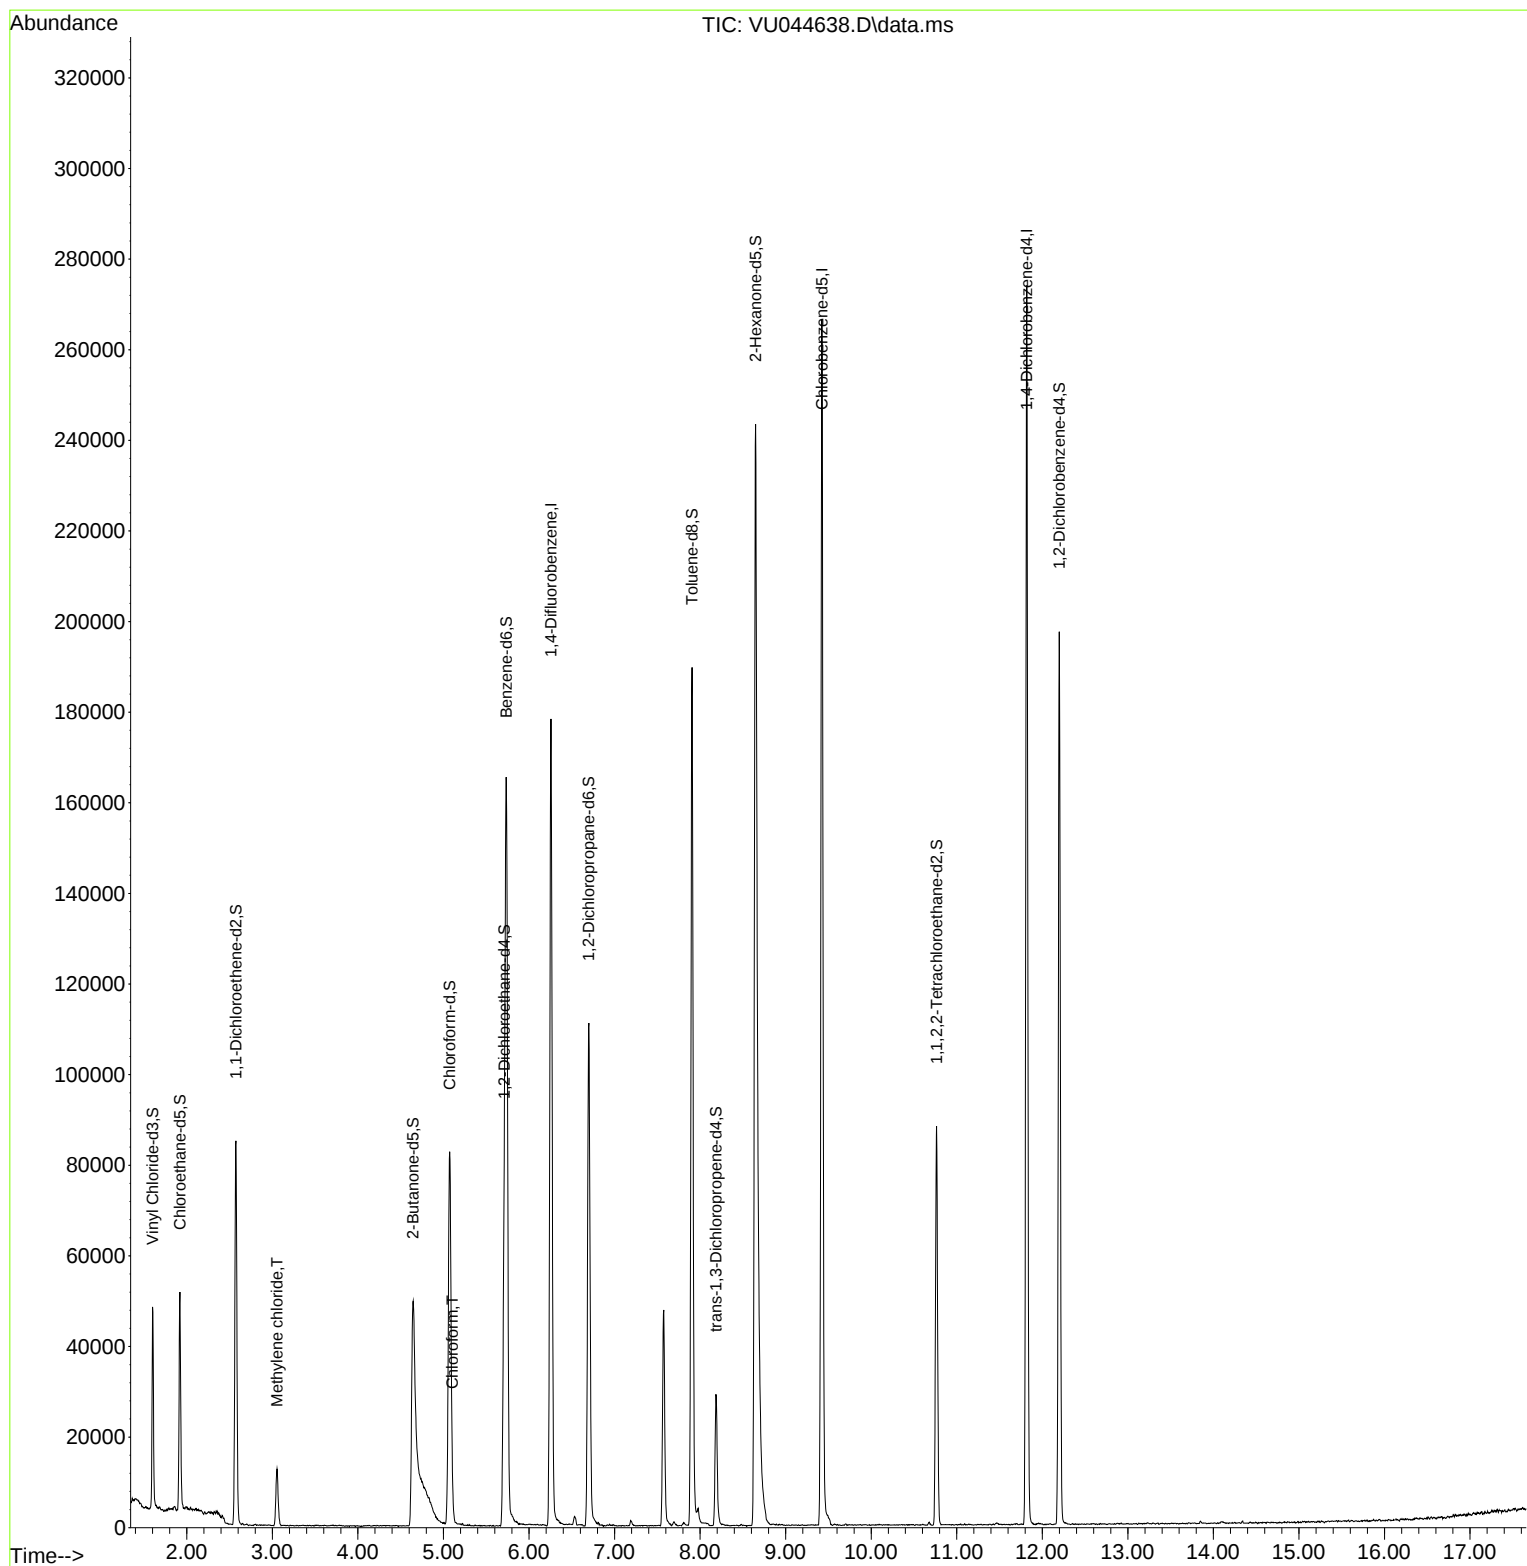

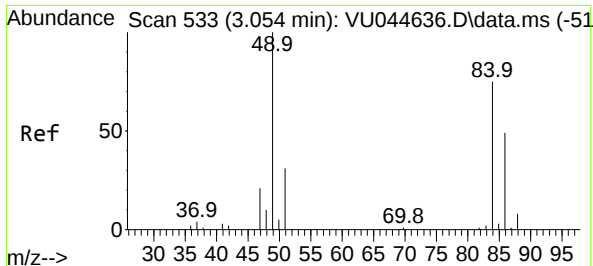

#16
Methylene chloride
Concen: 0.373 ug/L
RT: 3.054 min Scan# 533
Delta R.T. -0.000 min
Lab File: VU044638.D
Acq: 15 Sep 2021 12:16




Instrument :
MSVOA_U
ClientSampleId :
VBLK020

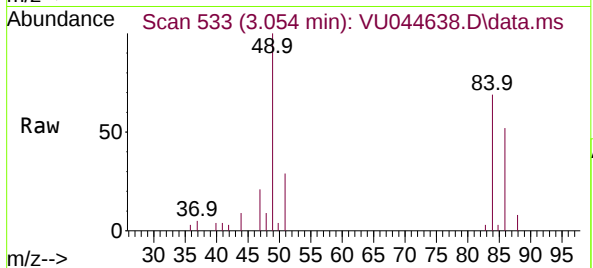


Tgt Ion: 84 Resp: 5257
Ion Ratio Lower Upper
84 100
86 76.1 45.8 85.2
49 151.0 92.9 172.5

Manual Integrations
APPROVED

MMDadoda
9/16/2021 12:12:48 PM

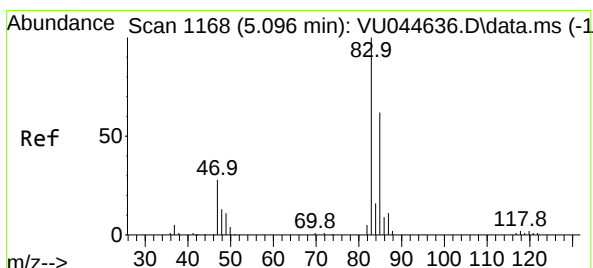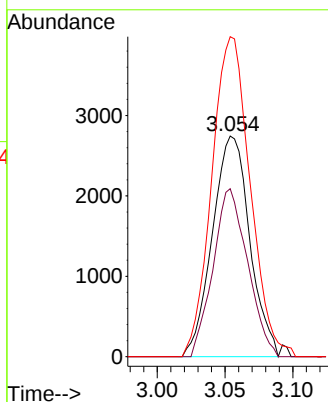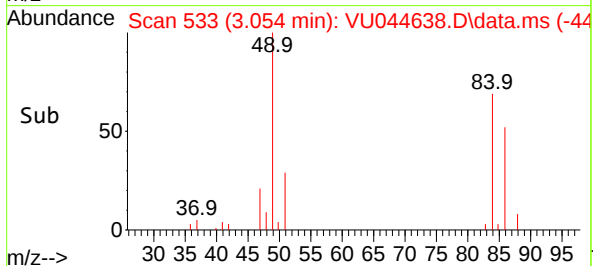

#25
Chloroform
Concen: 0.251 ug/L
RT: 5.102 min Scan# 1170
Delta R.T. 0.006 min
Lab File: VU044638.D
Acq: 15 Sep 2021 12:16

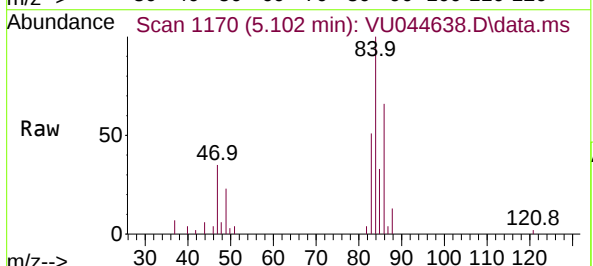

Tgt Ion: 83 Resp: 5097
Ion Ratio Lower Upper
83 100
85 64.7 44.2 82.0

