

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091521\
 Data File : VU044643.D
 Acq On : 15 Sep 2021 15:22
 Operator : SY/MD
 Sample : M3739-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B76

Quant Time: Sep 16 01:44:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 16 01:40:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	137083	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	140350	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	64631	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	29419	3.637	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.800%
7) Chloroethane-d5	1.919	69	34191	4.142	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.800%
11) 1,1-Dichloroethene-d2	2.572	65	15579	3.813	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.200%
20) 2-Butanone-d5	4.642	46	160171	47.239	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.480%
24) Chloroform-d	5.073	84	75794	4.455	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	5.710	65	46426	4.576	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
32) Benzene-d6	5.736	84	146637	4.098	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.000%
36) 1,2-Dichloropropane-d6	6.697	67	51597	4.390	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.800%
41) Toluene-d8	7.903	98	119274	3.829	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.600%
43) trans-1,3-Dichloroprop...	8.186	79	15716	3.794	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.800%
46) 2-Hexanone-d5	8.645	63	119266	44.793	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.580%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	44962	4.315	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.200%
66) 1,2-Dichlorobenzene-d4	12.198	152	45343	4.252	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.000%
Target Compounds					Qvalue	
13) Acetone	2.652	43	6159	2.789	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091521\
Data File : VU044643.D
Acq On : 15 Sep 2021 15:22
Operator : SY/MD
Sample : M3739-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B76


Quant Time: Sep 16 01:44:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 16 01:40:15 2021
Response via : Initial Calibration

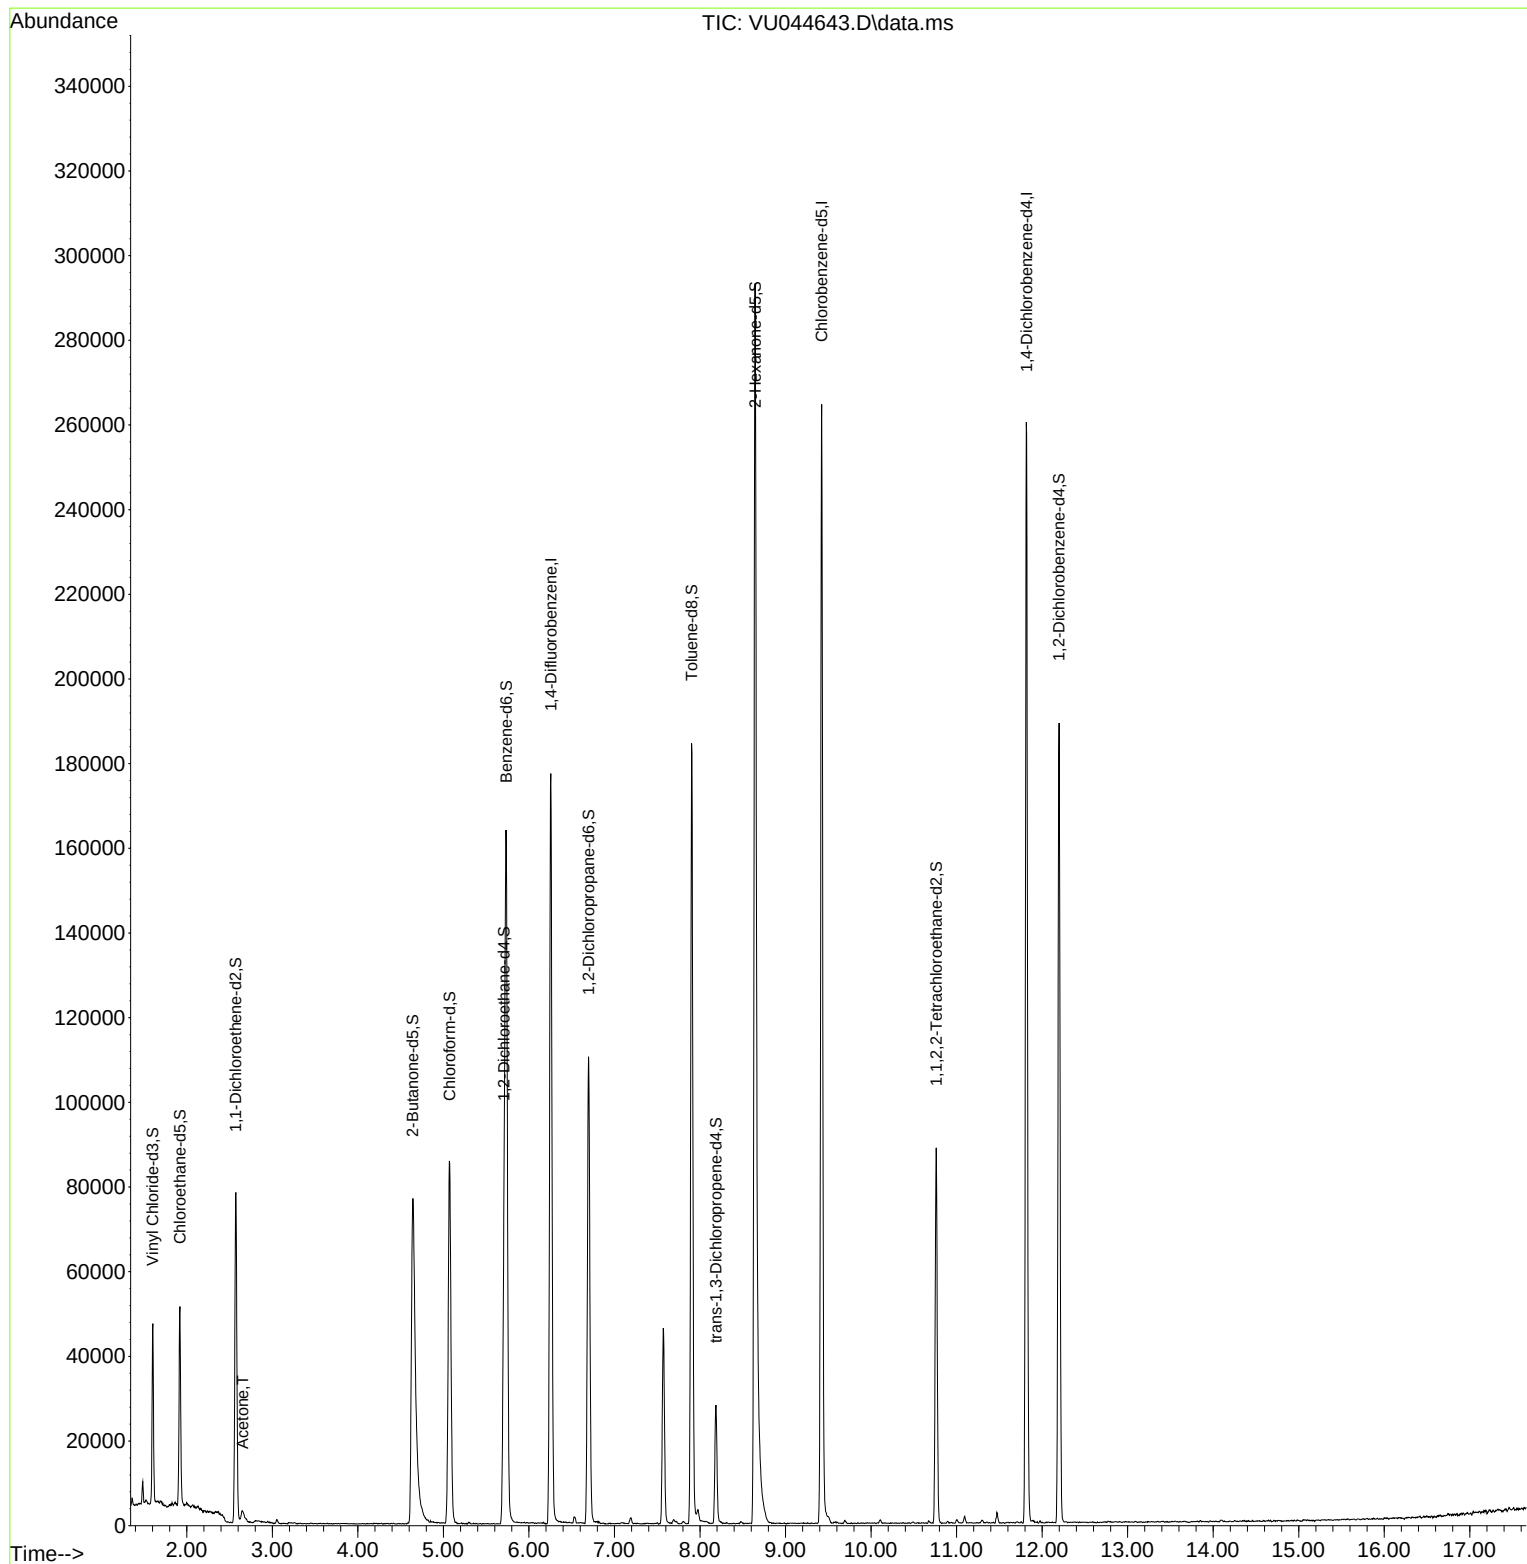

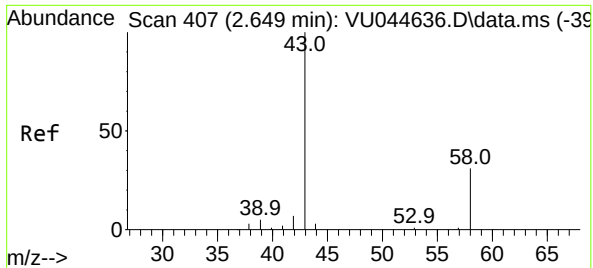

#13
 Acetone
 Concen: 2.789 ug/L
 RT: 2.652 min Scan# 408
 Delta R.T. 0.003 min
 Lab File: VU044643.D
 Acq: 15 Sep 2021 15:22

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B76

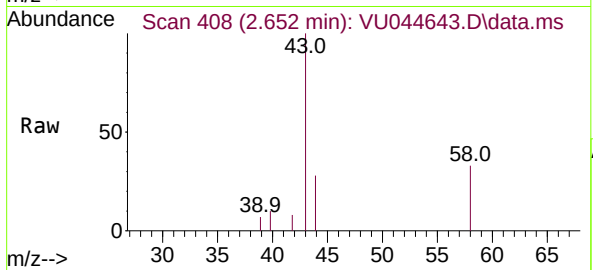

Tgt Ion: 43 Resp: 6159
 Ion Ratio Lower Upper
 43 100
 58 23.7 0.0 42.4

