

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091521\
 Data File : VU044644.D
 Acq On : 15 Sep 2021 15:56
 Operator : SY/MD
 Sample : M3739-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK1

Quant Time: Sep 16 01:44:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 16 01:40:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	136148	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	140860	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	65546	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	29166	3.631	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.600%
7) Chloroethane-d5	1.919	69	33956	4.142	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.800%
11) 1,1-Dichloroethene-d2	2.575	65	15565	3.836	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.800%
20) 2-Butanone-d5	4.645	46	157189	46.678	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.360%
24) Chloroform-d	5.073	84	76101	4.504	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%
26) 1,2-Dichloroethane-d4	5.710	65	45229	4.489	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.800%
32) Benzene-d6	5.735	84	146655	4.083	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.600%
36) 1,2-Dichloropropane-d6	6.700	67	52113	4.418	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.400%
41) Toluene-d8	7.906	98	119650	3.827	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.600%
43) trans-1,3-Dichloroprop...	8.185	79	15740	3.786	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.800%
46) 2-Hexanone-d5	8.645	63	114198	42.734	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.460%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	44066	4.213	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.200%
66) 1,2-Dichlorobenzene-d4	12.198	152	46822	4.329	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.600%
Target Compounds						
					Qvalue	
13) Acetone	2.649	43	5286	2.410	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091521\
Data File : VU044644.D
Acq On : 15 Sep 2021 15:56
Operator : SY/MD
Sample : M3739-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK1

Quant Time: Sep 16 01:44:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 16 01:40:15 2021
Response via : Initial Calibration

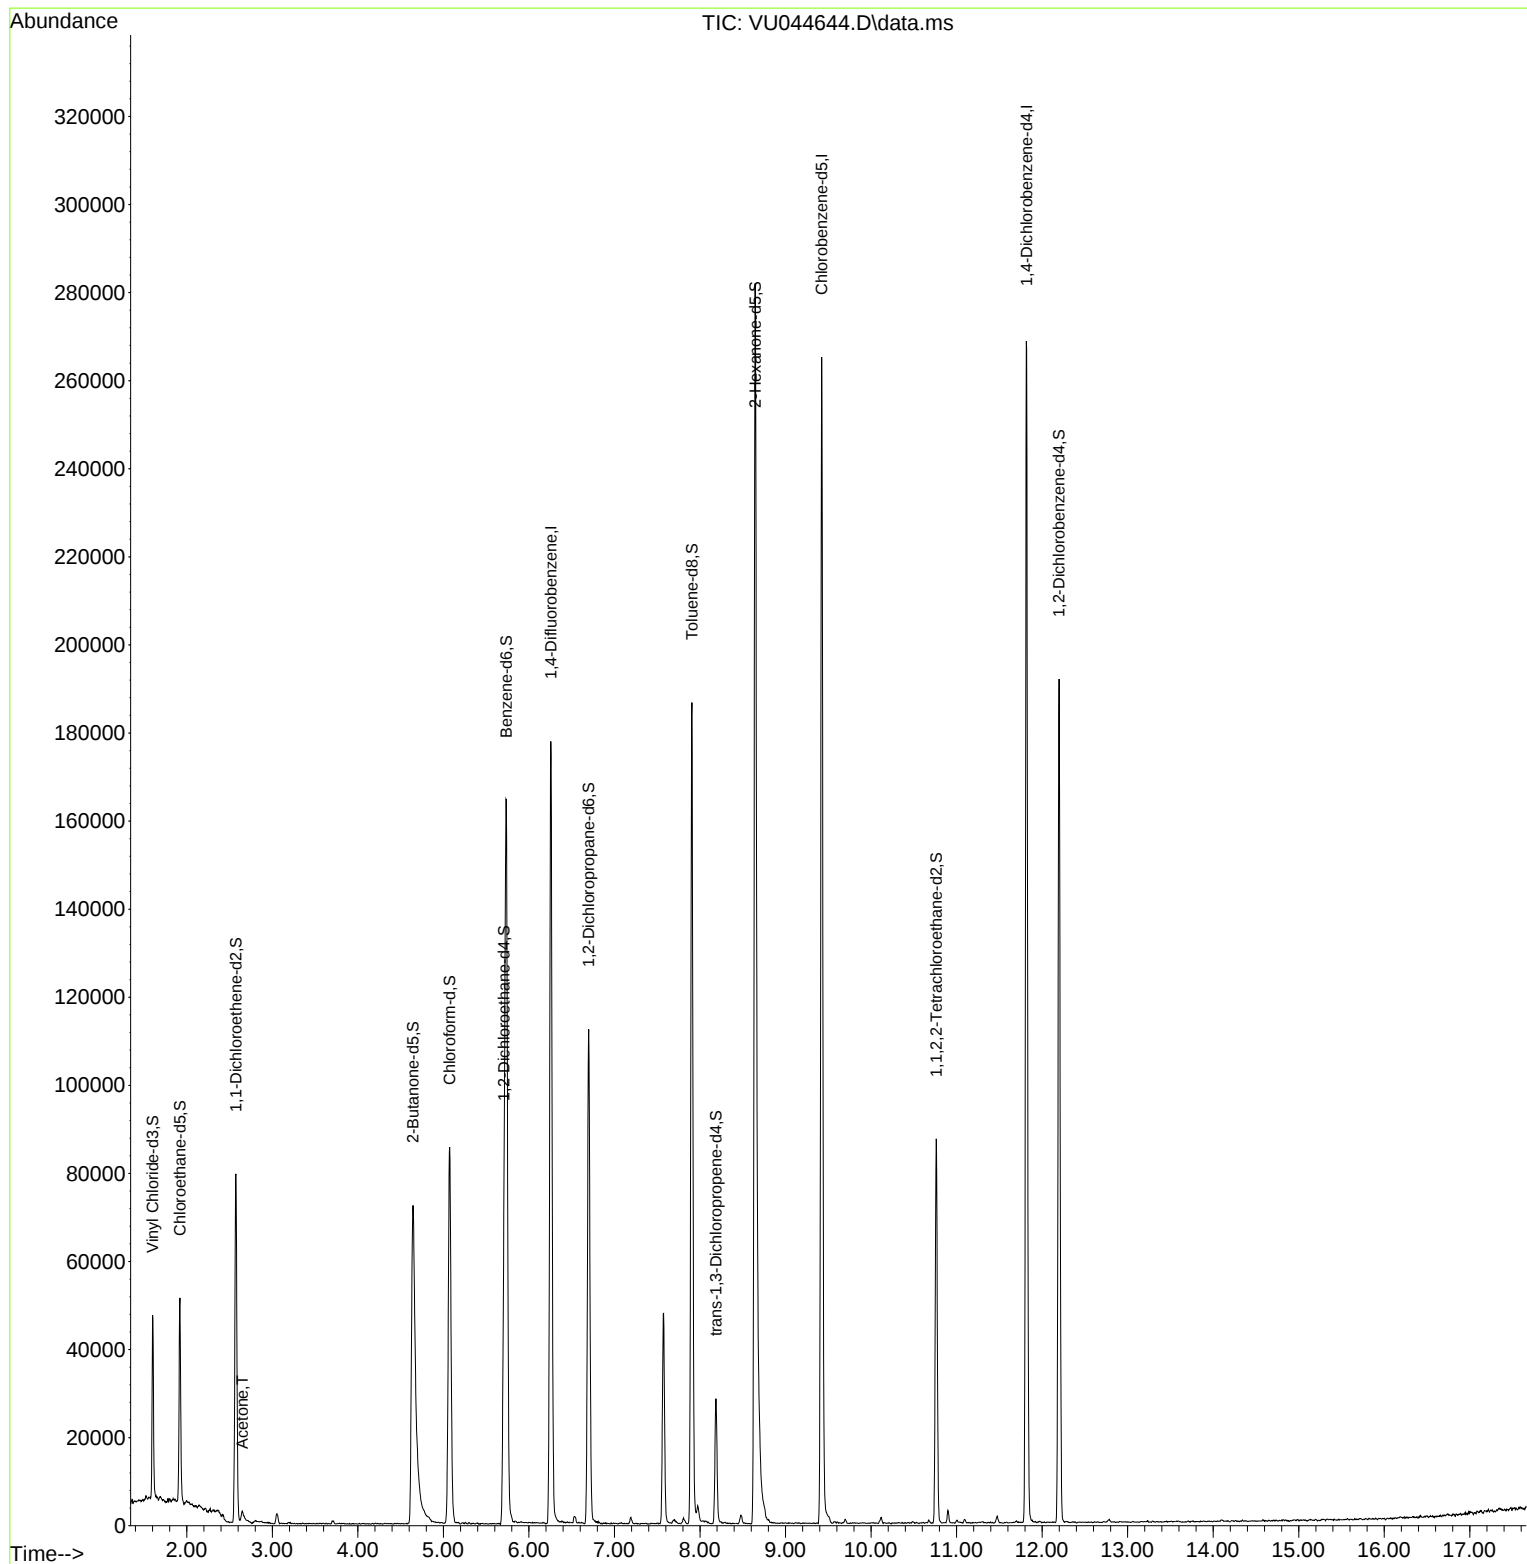

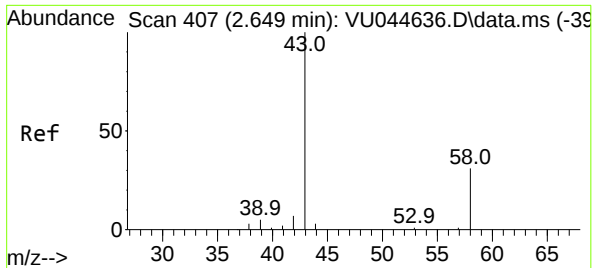

#13
 Acetone
 Concen: 2.410 ug/L
 RT: 2.649 min Scan# 407
 Delta R.T. -0.000 min
 Lab File: VU044644.D
 Acq: 15 Sep 2021 15:56

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK1

Tgt Ion:	43	Resp:	5286
Ion Ratio	Lower	Upper	
43	100		
58	17.5	0.0	42.4

