

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091521\
 Data File : VU044650.D
 Acq On : 15 Sep 2021 18:22
 Operator : SY/MD
 Sample : M3739-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B74

Quant Time: Sep 16 01:45:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 16 01:40:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	124119	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	126441	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	54932	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	27051	3.694	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.800%
7) Chloroethane-d5	1.916	69	32390	4.334	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.600%
11) 1,1-Dichloroethene-d2	2.572	65	14491	3.918	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.400%
20) 2-Butanone-d5	4.642	46	158389	51.593	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.180%
24) Chloroform-d	5.070	84	74648	4.846	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.000%
26) 1,2-Dichloroethane-d4	5.710	65	44200	4.812	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.200%
32) Benzene-d6	5.735	84	139964	4.341	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.800%
36) 1,2-Dichloropropane-d6	6.697	67	50246	4.746	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.000%
41) Toluene-d8	7.903	98	110642	3.942	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.800%
43) trans-1,3-Dichloroprop...	8.186	79	14664	3.929	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.600%
46) 2-Hexanone-d5	8.642	63	116872	48.722	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.440%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	44090	4.696	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.000%
66) 1,2-Dichlorobenzene-d4	12.198	152	41947	4.628	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.600%
Target Compounds						Qvalue
6) Bromomethane	1.861	94	481	0.077	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091521\
Data File : VU044650.D
Acq On : 15 Sep 2021 18:22
Operator : SY/MD
Sample : M3739-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B74


Quant Time: Sep 16 01:45:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 16 01:40:15 2021
Response via : Initial Calibration

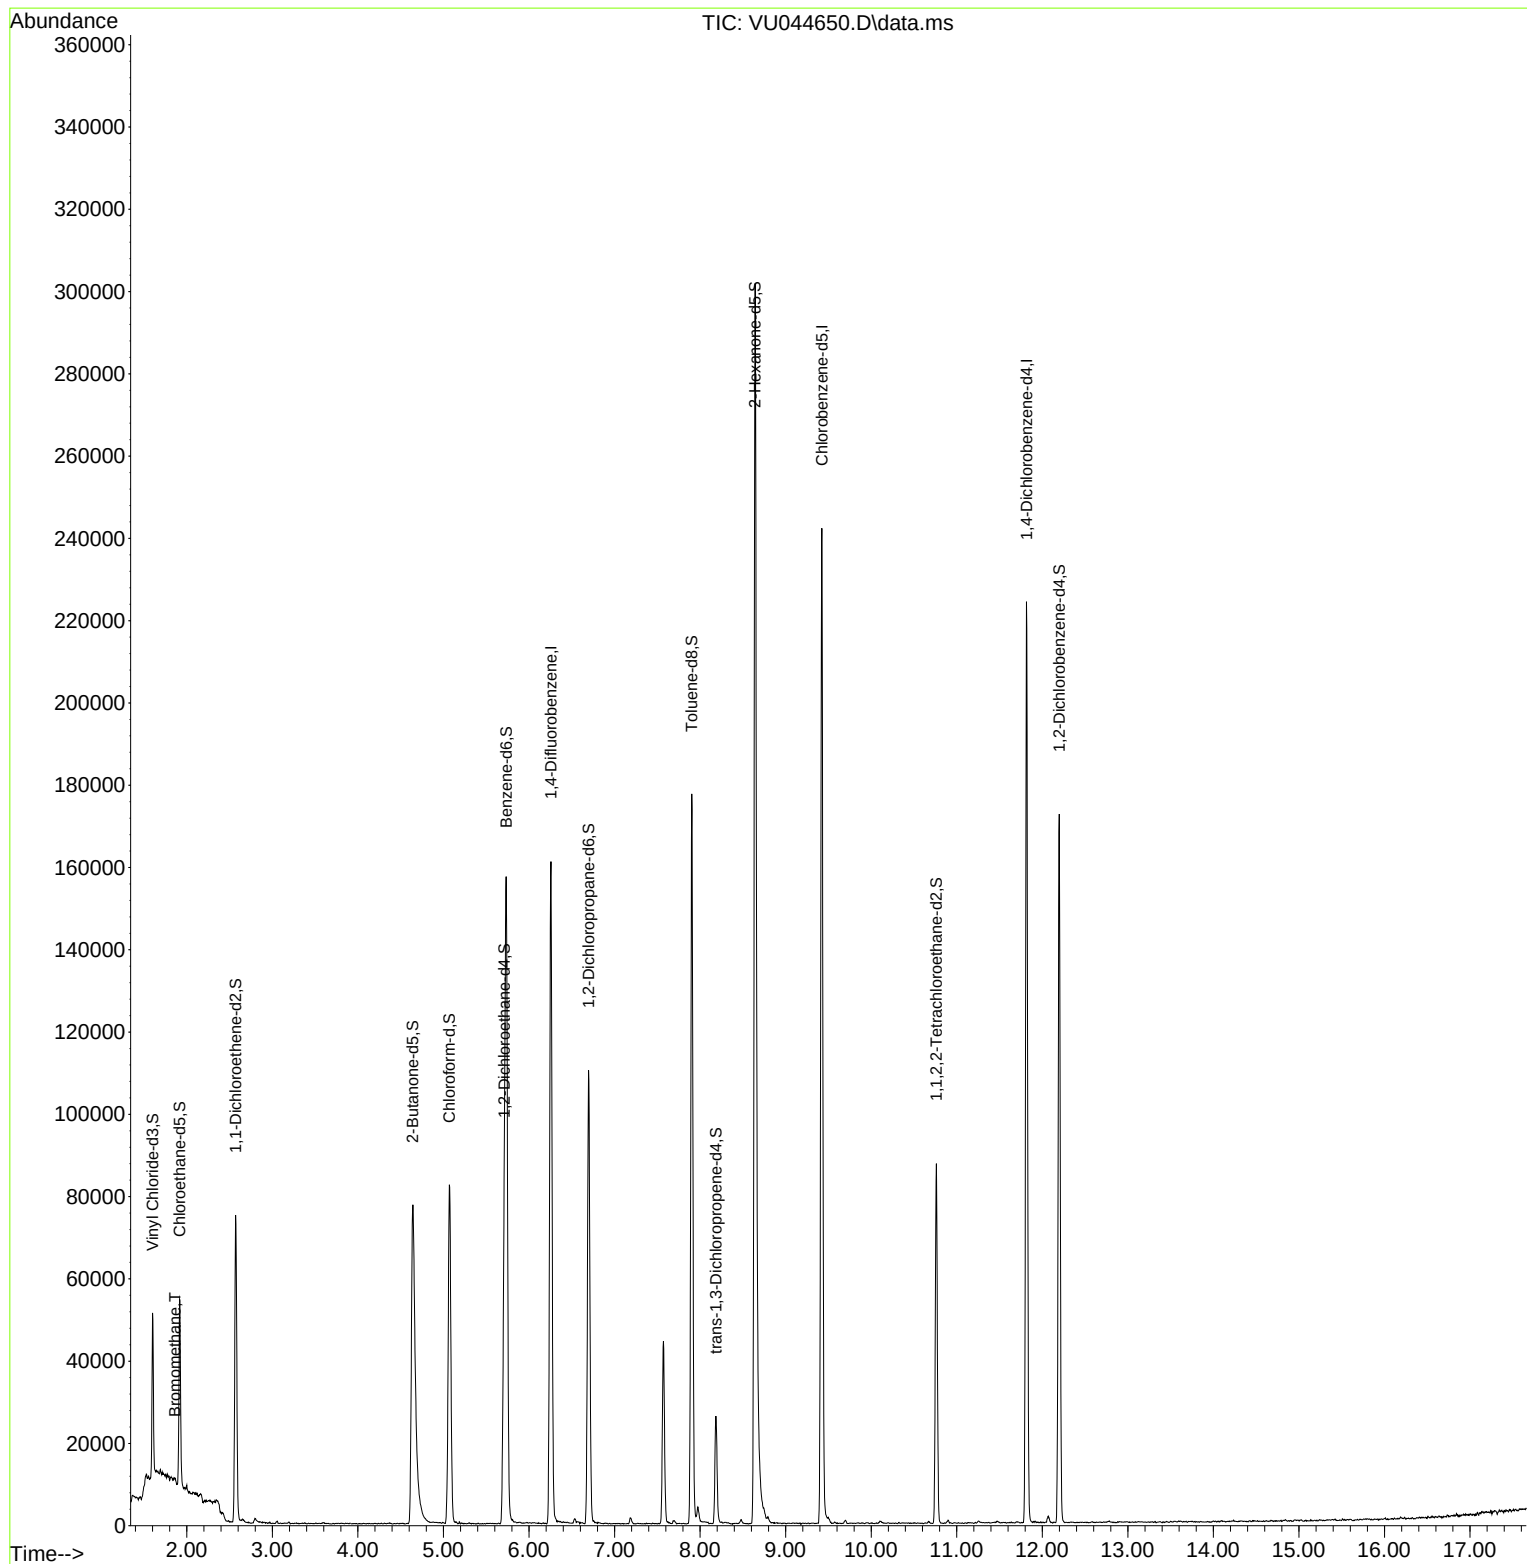

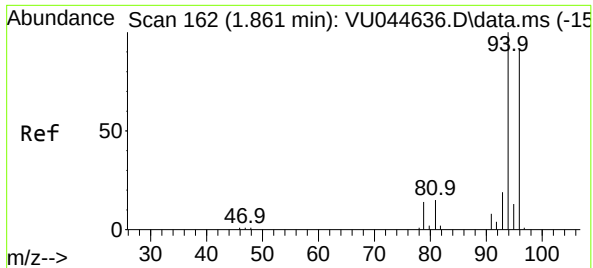

#6
Bromomethane
Concen: 0.077 ug/L
RT: 1.861 min Scan# 162
Delta R.T. 0.000 min
Lab File: VU044650.D
Acq: 15 Sep 2021 18:22

Instrument :
MSVOA_U
ClientSampleId :
C0B74

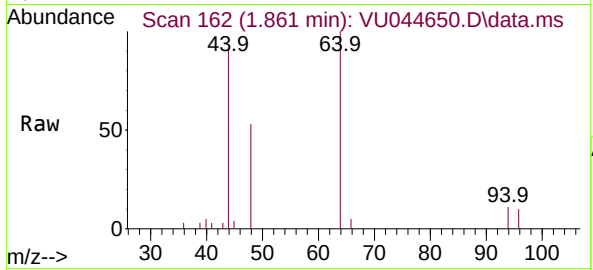

Tgt Ion: 94 Resp: 481
Ion Ratio Lower Upper
94 100
96 89.5 66.4 123.4

