
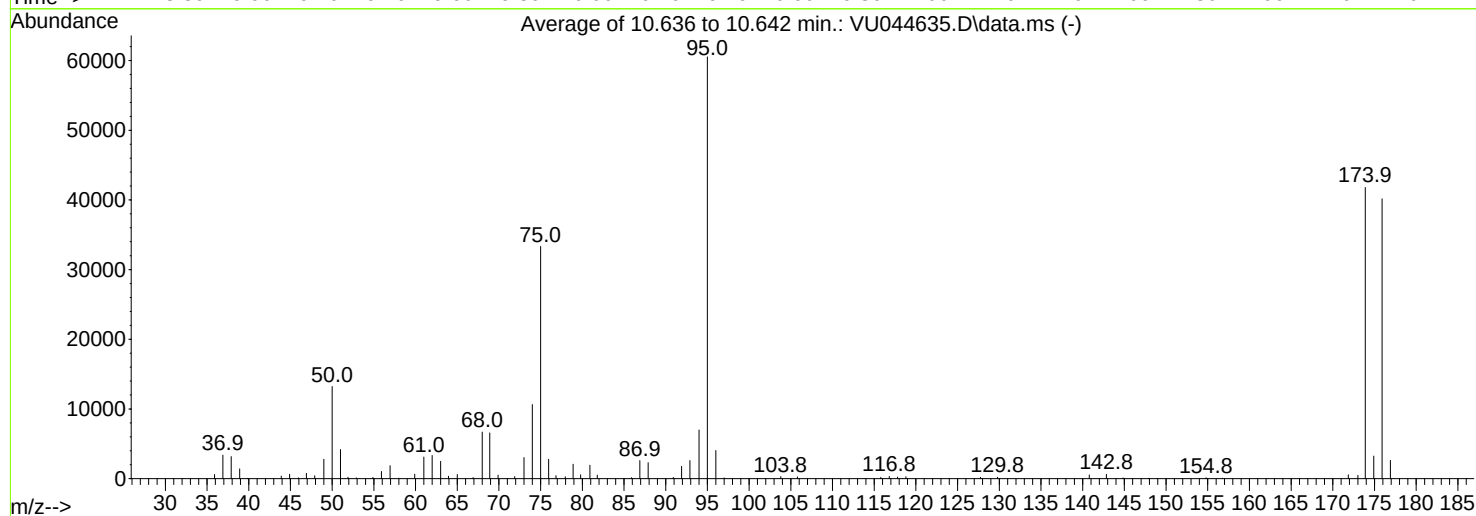


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091521\
 Data File : VU044635.D
 Acq On : 15 Sep 2021 09:10
 Operator : SY/MD
 Sample : BFB018
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB018

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Sep 23 02:59:45 2021

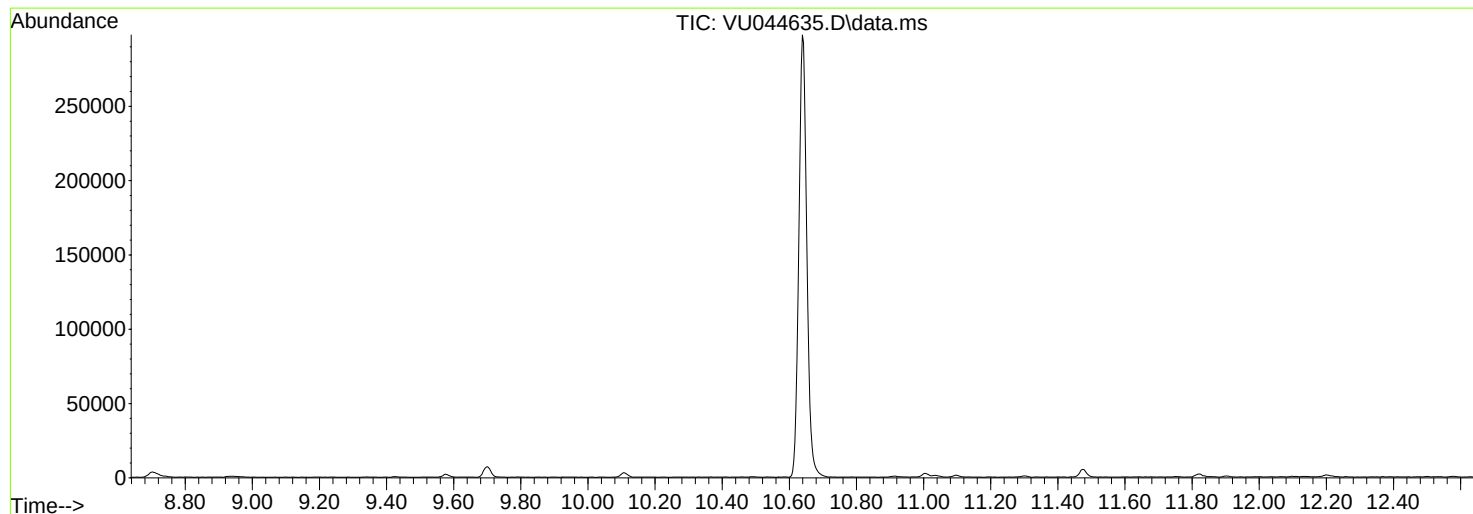

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	13228	PASS
75	95	30	80	55.0	33320	PASS
95	95	100	100	100.0	60539	PASS
96	95	5	9	6.7	4036	PASS
173	174	0.00	2	1.2	493	PASS
174	95	50	120	69.1	41803	PASS
175	174	5	9	7.7	3232	PASS
176	174	95	101	96.1	40163	PASS
177	176	5	9	6.5	2608	PASS

m/z	Abundance
39.80	160.0
43.90	361.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	610.0
36.90	3264.0
37.90	3119.0
38.90	1425.0
39.90	230.0
43.90	693.0
44.90	607.0
45.90	110.0
46.90	752.0
47.90	423.0
49.00	2697.0
50.00	13049.0
51.00	4189.0
51.90	204.0
52.90	107.0
54.90	181.0
55.90	1009.0
56.90	1813.0
59.90	636.0
61.00	3129.0
62.00	3292.0
63.00	2456.0
64.00	368.0
65.00	517.0
66.90	170.0
68.00	6369.0
68.90	6413.0
69.90	582.0
71.90	264.0
73.00	2951.0
74.00	10300.0
75.00	32080.0
76.00	2790.0
76.90	435.0
78.00	219.0
78.90	2071.0
79.80	557.0
80.90	1783.0
81.80	465.0
85.90	130.0
86.90	2590.0
87.90	2213.0
90.90	179.0
91.90	1643.0
92.90	2572.0
94.00	6675.0
95.00	57976.0
96.00	3884.0
97.00	112.0
103.80	245.0
105.80	283.0
115.80	155.0
116.80	327.0
117.80	212.0
118.80	274.0
127.80	189.0
129.80	203.0
140.80	559.0
142.90	576.0
144.80	124.0
154.80	138.0
156.80	105.0
171.80	501.0
173.00	462.0
173.90	39000.0
174.90	2992.0
175.90	37016.0
176.90	2459.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	601.0
36.90	3463.0
37.90	3220.0
38.90	1473.0
39.90	221.0
43.90	756.0
44.90	614.0
46.00	130.0
46.90	790.0
47.90	441.0
49.00	2847.0
50.00	13642.0
51.00	4299.0
51.90	207.0
52.90	114.0
54.90	185.0
55.90	1063.0
57.00	1912.0
58.00	115.0
59.90	662.0
61.00	3224.0
62.00	3446.0
63.00	2540.0
63.90	343.0
65.00	627.0
66.90	147.0
68.00	6866.0
68.90	6725.0
69.90	513.0
71.90	305.0
73.00	3142.0
74.00	10947.0
75.00	34528.0
75.90	2863.0
76.80	454.0
78.00	263.0
78.90	2135.0
79.80	555.0
80.90	1971.0
81.80	514.0
85.90	137.0
86.90	2693.0
87.90	2359.0
90.90	199.0
91.90	1828.0
92.90	2637.0
94.00	7144.0
95.00	62616.0
96.00	4122.0
97.00	128.0
103.80	305.0
105.80	273.0
115.80	196.0
116.80	320.0
117.80	237.0
118.80	279.0
127.80	174.0
129.80	225.0
140.80	540.0
142.80	649.0
144.80	117.0
154.80	139.0
156.70	105.0
171.80	571.0
173.00	515.0
173.90	43032.0
174.90	3353.0
175.90	41496.0
176.90	2670.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	591.0
36.90	3406.0
37.90	3149.0
38.90	1333.0
39.90	199.0
43.90	771.0
44.90	613.0
46.00	128.0
46.90	739.0
47.90	404.0
49.00	2821.0
50.00	12994.0
51.00	4062.0
51.90	211.0
52.90	100.0
54.90	176.0
55.90	1003.0
57.00	1853.0
58.00	113.0
59.90	653.0
61.00	2980.0
62.00	3252.0
63.00	2464.0
64.00	306.0
65.00	682.0
66.90	144.0
68.00	6784.0
68.90	6578.0
69.90	438.0
71.90	328.0
73.00	3026.0
74.00	10630.0
75.00	33352.0
75.90	2707.0
76.90	392.0
77.90	324.0
78.90	2013.0
79.80	536.0
80.90	2033.0
81.80	515.0
85.90	121.0
86.90	2529.0
87.90	2347.0
90.90	192.0
91.90	1824.0
92.90	2589.0
94.00	7148.0
95.00	61024.0
96.00	4101.0
97.00	119.0
103.80	316.0
105.80	235.0
115.80	207.0
116.80	322.0
117.80	224.0
118.80	297.0
127.70	159.0
129.80	218.0
140.80	490.0
142.80	665.0
144.90	106.0
147.90	108.0
154.80	117.0
171.90	569.0
173.00	502.0
173.90	43376.0
174.90	3352.0
175.90	41976.0
176.90	2695.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018