

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091523\
 Data File : VU055342.D
 Acq On : 15 Sep 2023 16:25
 Operator : MD/SY
 Sample : VU0915WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK037

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091523WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU055342.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	110	rBV	68081	95504	11.23%	1.437%
2	1.907	183	192	209	rBV	108312	216525	25.46%	3.258%
3	2.554	381	393	410	rVB	131175	214877	25.26%	3.233%
4	3.036	532	543	556	rBV2	17476	31512	3.71%	0.474%
5	4.634	1028	1040	1070	rBV	98294	323870	38.08%	4.873%
6	5.055	1155	1171	1199	rBV	151020	340319	40.01%	5.120%
7	5.718	1358	1377	1407	rBV3	278823	744967	87.59%	11.209%
8	6.245	1528	1541	1561	rBV	269756	517097	60.80%	7.780%
9	6.531	1618	1630	1643	rBV7	11760	25196	2.96%	0.379%
10	6.685	1661	1678	1696	rBV	181261	364187	42.82%	5.480%
11	7.563	1940	1951	1973	rBV2	81933	148223	17.43%	2.230%
12	7.894	2042	2054	2072	rBV	298215	530980	62.43%	7.989%
13	7.968	2072	2077	2095	rVB7	5706	12378	1.46%	0.186%
14	8.177	2130	2142	2163	rBV2	48424	88677	10.43%	1.334%
15	8.647	2273	2288	2326	rBV2	288515	850496	100.00%	12.797%
16	9.415	2514	2527	2556	rBV	393886	672320	79.05%	10.116%
17	10.113	2732	2744	2757	rBV8	5275	13002	1.53%	0.196%
18	10.759	2930	2945	2959	rBV	134672	229459	26.98%	3.452%
19	11.473	3158	3167	3180	rVB3	6278	10701	1.26%	0.161%
20	11.750	3244	3253	3261	rBV3	6540	9265	1.09%	0.139%
21	11.811	3261	3272	3295	rVV	395500	647674	76.15%	9.745%
22	12.193	3378	3391	3411	rBV	293487	492206	57.87%	7.406%
23	13.225	3704	3712	3727	rBV6	6813	11342	1.33%	0.171%
24	13.843	3896	3904	3914	rBV4	12117	18861	2.22%	0.284%
25	14.093	3970	3982	3995	rBV2	9134	18913	2.22%	0.285%
26	14.331	4046	4056	4072	rBV4	10745	17698	2.08%	0.266%




Sum of corrected areas: 6646249

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091523\
Data File : VU055342.D
Acq On : 15 Sep 2023 16:25
Operator : MD/SY
Sample : VU0915WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091523WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

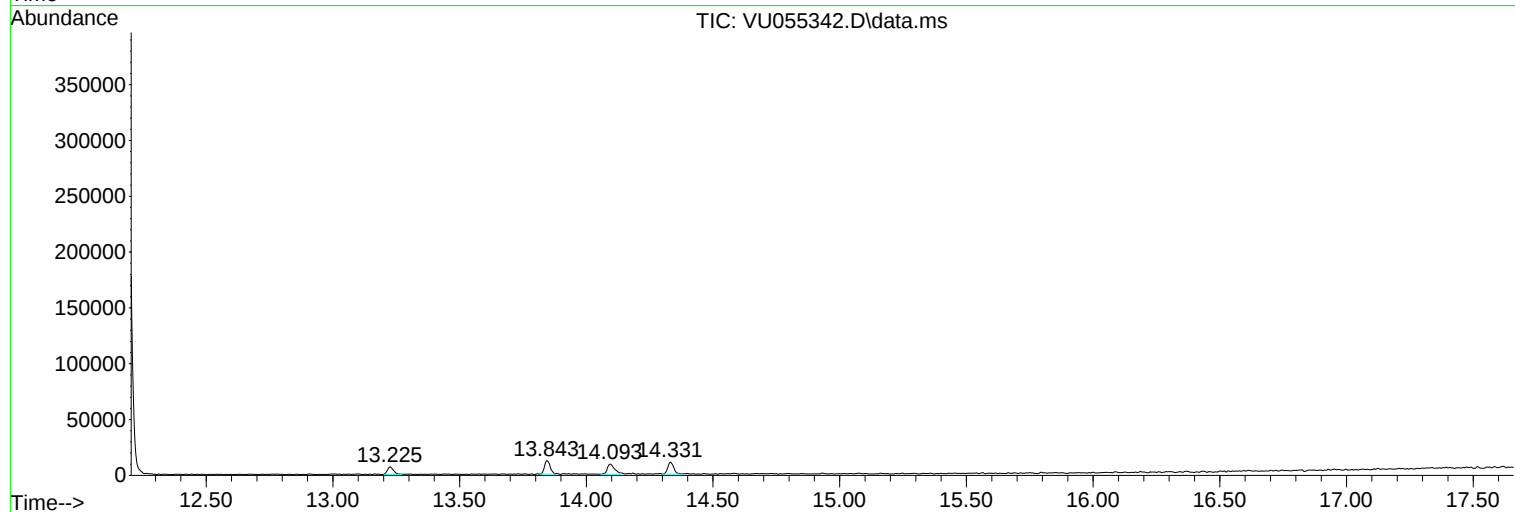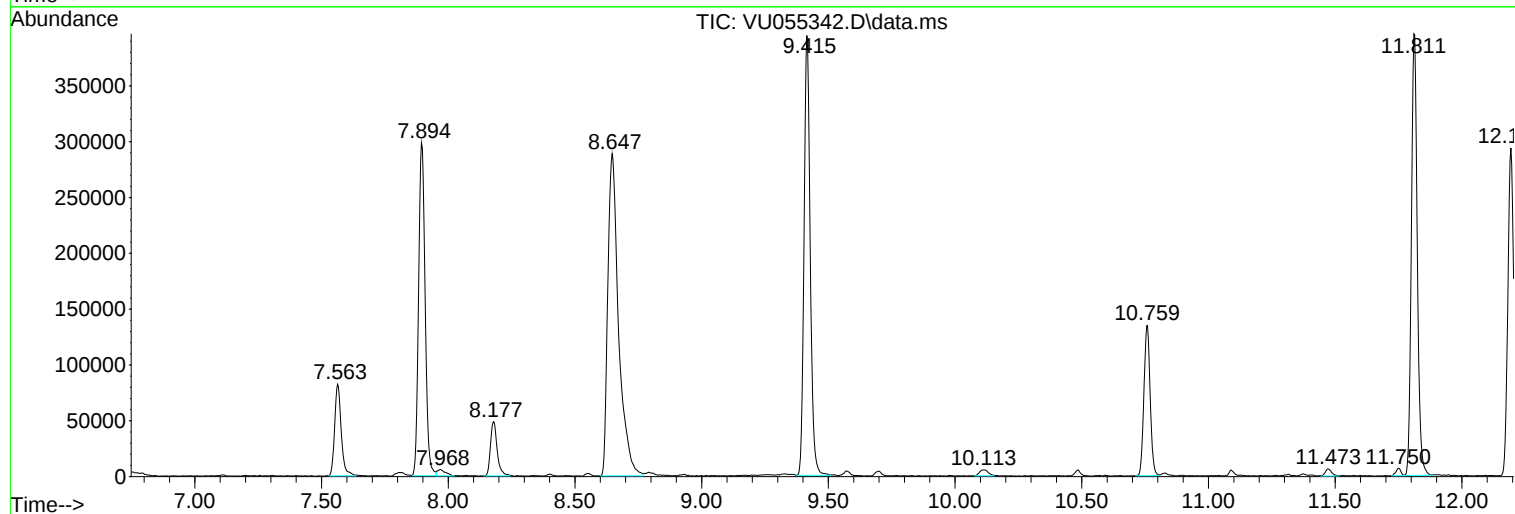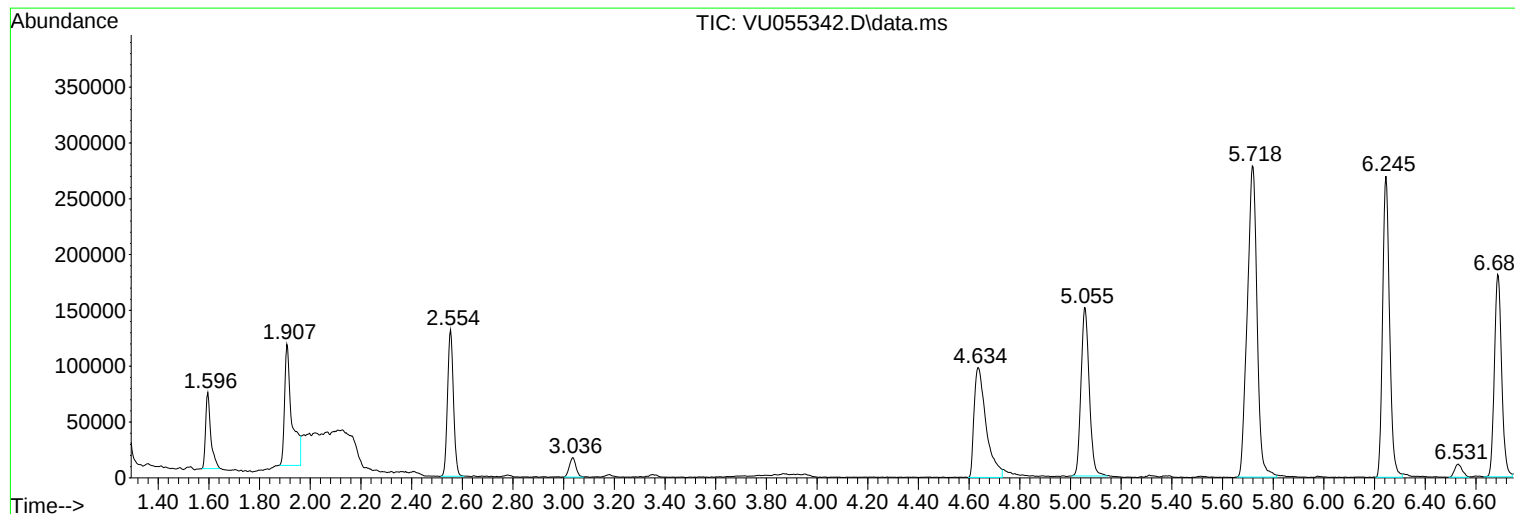

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091523\
Data File : VU055342.D
Acq On : 15 Sep 2023 16:25
Operator : MD/SY
Sample : VU0915WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091523WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091523\
Data File : VU055342.D
Acq On : 15 Sep 2023 16:25
Operator : MD/SY
Sample : VU0915WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091523WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc