
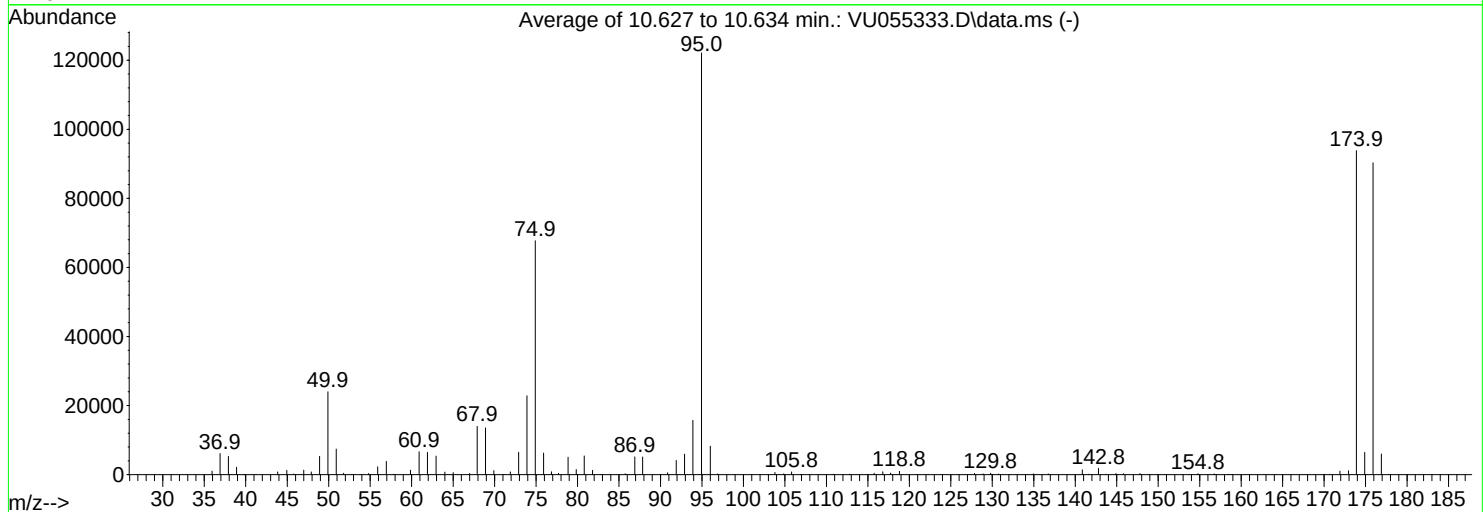


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091523\
Data File : VU055333.D
Acq On : 15 Sep 2023 10:13
Operator : MD/SY
Sample : BFB045
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB045

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091523WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Sep 19 01:12:51 2023

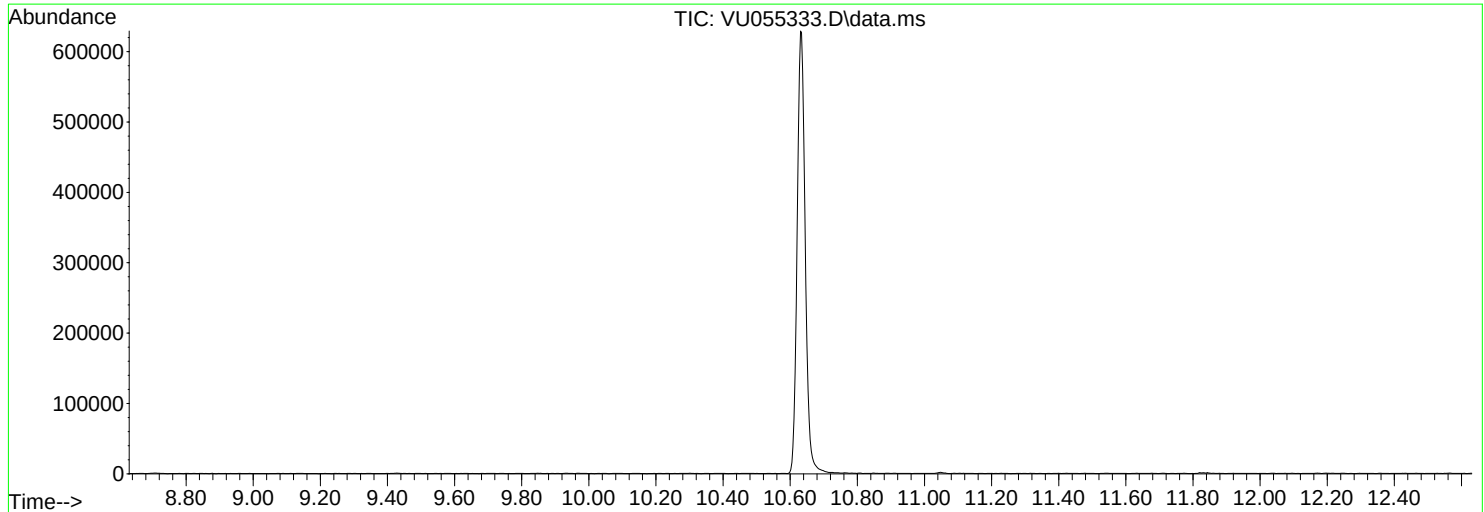

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	24003	PASS
75	95	30	80	55.5	67752	PASS
95	95	100	100	100.0	122133	PASS
96	95	5	9	6.8	8257	PASS
173	174	0.00	2	1.2	1111	PASS
174	95	50	120	76.8	93837	PASS
175	174	5	9	6.9	6442	PASS
176	174	95	101	96.3	90320	PASS
177	176	5	9	6.6	5987	PASS

m/z	Abundance
39.80	194.0
43.80	498.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.90	1076.0
36.90	5613.0
37.90	4844.0
38.90	2164.0
39.80	180.0
43.90	1299.0
44.90	1205.0
45.70	169.0
47.00	1310.0
47.90	714.0
48.90	5046.0
49.90	22696.0
50.90	7152.0
51.80	424.0
54.80	272.0
55.90	2127.0
57.00	3704.0
57.90	142.0
59.80	1223.0
60.90	6608.0
61.90	6293.0
63.00	5380.0
64.00	688.0
65.00	620.0
67.00	292.0
67.90	13626.0
68.90	12453.0
69.90	1026.0
71.90	702.0
72.90	6185.0
73.90	21920.0
74.90	65352.0
75.90	5943.0
76.80	668.0
77.80	371.0
78.90	4786.0
79.80	1547.0
80.80	4969.0
81.80	1187.0
85.90	323.0
86.90	4911.0
87.80	4657.0
90.80	520.0
91.90	3632.0
92.90	5762.0
93.90	14785.0
94.90	115464.0
96.00	7912.0
96.90	243.0
103.80	578.0
104.80	204.0
105.80	792.0
110.80	204.0
112.80	126.0
115.80	432.0
116.80	779.0
117.80	413.0
118.80	922.0
127.80	460.0
128.90	181.0
129.80	315.0
130.70	168.0
135.00	218.0
136.70	192.0
140.80	1345.0
141.60	117.0
142.80	1688.0
144.90	331.0
145.80	268.0
147.80	352.0
148.90	166.0
154.80	183.0
156.70	207.0
158.50	109.0
158.90	108.0
170.70	158.0
171.90	801.0
173.00	976.0
173.90	85416.0
174.90	6250.0
175.90	83504.0
176.90	5598.0
177.80	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
36.00	1070.0
36.90	6395.0
37.90	5490.0
38.90	2180.0
39.80	217.0
43.90	1289.0
44.90	1349.0
45.80	187.0
47.00	1337.0
47.90	797.0
48.90	5422.0
49.90	24720.0
50.90	7657.0
51.80	428.0
54.80	282.0
55.90	2385.0
56.90	3923.0
57.90	140.0
59.80	1361.0
60.90	6820.0
61.90	6755.0
63.00	5559.0
64.00	805.0
65.00	598.0
67.00	335.0
67.90	14548.0
68.90	13929.0
69.90	1159.0
71.90	765.0
72.90	6763.0
73.90	23600.0
74.90	69920.0
75.90	6501.0
76.80	857.0
77.70	424.0
78.80	5155.0
79.90	1572.0
80.80	5591.0
81.80	1270.0
85.70	310.0
86.90	5317.0
87.80	5335.0
90.90	557.0
91.90	4296.0
92.90	6085.0
93.90	16256.0
95.00	126160.0
96.00	8499.0
96.90	244.0
103.80	626.0
104.90	242.0
105.80	821.0
110.80	165.0
112.80	135.0
115.70	415.0
116.80	895.0
117.80	477.0
118.80	1004.0
127.80	390.0
128.90	253.0
129.80	403.0
130.80	213.0
135.00	229.0
136.70	231.0
140.80	1410.0
141.60	157.0
142.80	1879.0
143.70	117.0
144.90	334.0
145.80	323.0
147.80	373.0
148.90	130.0
149.90	108.0
154.80	273.0
156.80	252.0
158.50	123.0
158.90	101.0
170.00	100.0
170.70	122.0
171.90	1045.0
173.00	1144.0
173.90	96464.0
174.90	6519.0
175.90	93008.0
176.90	6174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.90	873.0
36.90	6363.0
37.90	5473.0
38.90	2093.0
39.80	234.0
43.90	1253.0
45.00	1190.0
45.90	224.0
47.00	1286.0
47.90	850.0
48.90	5335.0
49.90	24592.0
50.90	7469.0
51.80	345.0
52.80	113.0
54.80	371.0
55.90	2310.0
56.90	3880.0
57.80	145.0
59.90	1322.0
60.90	6419.0
61.90	6299.0
62.90	5227.0
64.00	736.0
65.00	628.0
67.00	327.0
67.90	13855.0
68.90	14223.0
69.90	1279.0
71.90	839.0
72.90	6460.0
73.90	22944.0
74.90	67984.0
75.90	6338.0
76.90	926.0
77.60	381.0
78.80	5201.0
79.90	1393.0
80.80	5719.0
81.80	1255.0
82.80	100.0
85.70	212.0
86.90	5215.0
87.90	5358.0
90.90	537.0
91.90	4409.0
92.90	5992.0
93.90	16124.0
95.00	124776.0
96.00	8361.0
96.90	229.0
103.80	680.0
104.90	258.0
105.80	791.0
106.90	112.0
110.80	119.0
112.80	159.0
115.80	449.0
116.80	897.0
117.70	509.0
118.80	993.0
127.90	336.0
128.90	269.0
129.80	482.0
130.80	228.0
134.90	235.0
136.80	258.0
140.90	1390.0
141.70	210.0
142.80	1847.0
143.70	157.0
144.90	310.0
145.80	296.0
147.80	302.0
149.90	113.0
153.70	100.0
154.80	324.0
156.80	261.0
158.90	129.0
170.10	127.0
171.90	1191.0
172.90	1212.0
173.90	99632.0
174.90	6557.0
175.90	94448.0
176.90	6188.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045